

## Alu Positive Control Probe

**REF** 800-2845  
05278694001

**IVD**  $\Sigma$  50

### INTENDED USE

Alu Positive Control Probe is a cocktail of oligonucleotide probes labeled with fluorescein that is intended for the laboratory use as a positive control to determine the preservation of DNA during specimen collection, processing, fixation and handling, in sections of formalin-fixed, paraffin-embedded tissue on a BenchMark IHC/ISH instrument.

This product should be interpreted by a qualified pathologist in conjunction with histological examination, relevant clinical information, and proper controls.

This product is intended for in vitro diagnostic (IVD) use.

### SUMMARY AND EXPLANATION

The intended target of Alu Positive Control Probe is the Alu repeat DNA sequence found in the nuclei of cells in all tissue. Alu Positive Control Probe is useful to determine the preservation of DNA during specimen collection, processing, fixation and handling.

Alu Positive Control Probe should be run during assay verification and troubleshooting since DNA accessibility may vary depending on fixation method and pretreatment of the specimen.

### PRINCIPLE OF THE PROCEDURE

Alu Positive Control Probe is optimally formulated for use with VENTANA ISH MIEW Blue Detection Kit and accessory reagents on BenchMark IHC/ISH instruments.

During the Blue ISH staining process, the fluorescein labeled probe is hybridized to specific target DNA sequences in tissues. The anti-fluorescein antibody is followed by the addition of a biotinylated goat anti-mouse antibody. This step is followed by the addition of a Streptavidin-AP (alkaline phosphatase) enzyme conjugate which binds to the biotin present on the secondary antibody. The fluorescein labeled probe is then visualized with 5-Bromo-4-chloro-3-indolyl phosphate (BCIP) and nitro blue tetrazolium (NBT) chromogen, which produces a blue precipitate. The specimen may then be counterstained and cover slipped. Results are interpreted using a light microscope. Alu Positive Control Probe is used with VENTANA detection reagents and accessory reagents, and a BenchMark IHC/ISH instrument as a control in ISH staining applications.

Figure 1 illustrates the Blue ISH reaction.

### MATERIAL PROVIDED

Alu Positive Control Probe contains sufficient reagent for 50 tests.

One 5 mL dispenser of Alu Positive Control Probe contains approximately 500 ng/mL of the probe labeled with fluorescein, formulated in a formamide-based hybridization buffer. Refer to the appropriate VENTANA detection kit method sheet for detailed descriptions of: Principles of the Procedure, Materials and Methods, Specimen Collection and Preparation for Analysis, Quality Control Procedures, Troubleshooting, Interpretation of Results, and Limitations.

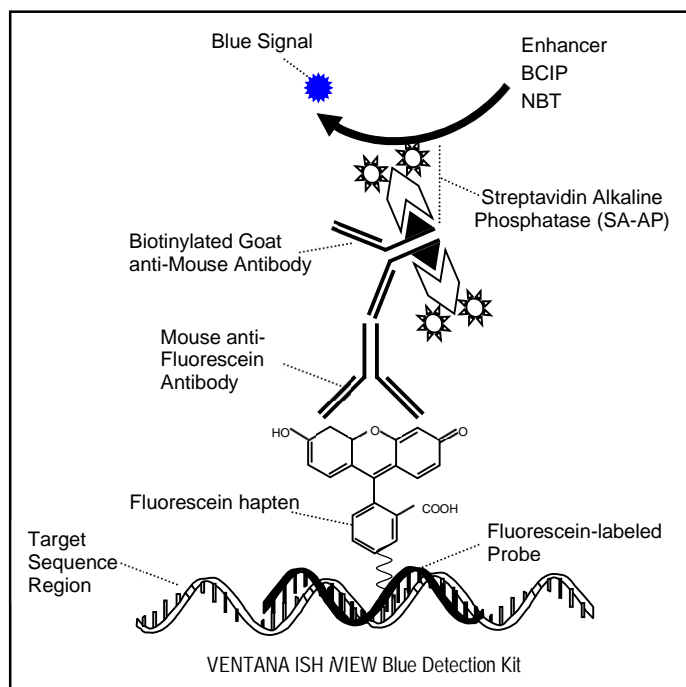


Figure 1. Blue ISH Reaction.

### MATERIALS REQUIRED BUT NOT PROVIDED

Staining reagents, such as VENTANA detection kits and ancillary components, including negative and positive tissue control slides, are not provided.

Not all products listed in the method sheet may be available in all geographies. Consult your local support representative.

The following reagents and materials may be required for staining but are not provided with the probe:

1. VENTANA ISH MIEW Blue Detection Kit (Cat. No. 800-092 / 05278511001)
2. ISH Protease 3 (Cat. No. 780-4149 / 05273331001)
3. Red Counterstain II (Cat. No. 780-2218 / 05272017001)
4. Reaction Buffer Concentrate (10X) (Cat. No. 950-300 / 05353955001)
5. 10X SSC (Cat. No. 950-110 / 05353947001)
6. EZ Prep Concentrate (10X) (Cat. No. 950-102 / 05279771001)
7. ULTRA Cell Conditioning (ULTRA CC2) (Cat. No. 950-223 / 05424542001)
8. LCS (Low Temperature) (Cat. No. 250-009 / 05260981001)
9. ULTRA LCS (Predilute) (Cat. No. 650-210 / 05424534001)
10. Microscope slides, positively charged
11. BenchMark IHC/ISH instrument
12. General purpose laboratory equipment

### STORAGE AND STABILITY

Upon receipt and when not in use, store at 2-8 °C. Do not freeze.

To ensure proper reagent delivery and the stability of the antibody, replace the dispenser cap after every use and immediately place the dispenser in the refrigerator in an upright position.

Every probe dispenser is expiration dated. When properly stored, the reagent is stable to the date indicated on the label. Do not use reagent beyond the expiration date.

### SPECIMEN PREPARATION

Routinely processed, formalin-fixed, paraffin-embedded tissues are suitable for use with this probe when used with a BenchMark IHC/ISH instrument. The recommended tissue fixative is 10% neutral buffered formalin.<sup>1</sup> Slides should be stained immediately, as quality of nucleic acid targets in cut tissue sections may diminish over time.

It is recommended that positive and negative controls be run simultaneously with unknown specimens.

Sections thicker than 4 µm may require stronger protease treatment than the recommended condition and may exhibit more nuclear bubbling than thinner sections due to excess paraffin in the tissue. Nuclear bubbling appears as large or small bubbles or vacuoles in the nuclei. Usually this artifact does not interfere with signal enumeration. However, severe cases of nuclear bubbling may distort the nuclei or signals such that enumeration is not possible. These specimens may need to be deparaffinized in xylene and alcohol baths prior to repeat staining on the instrument, or the user may select the extended deparaffinization option in the staining procedure (see Troubleshooting).

**WARNINGS AND PRECAUTIONS**

- For in vitro diagnostic (IVD) use.
- For professional use only.
- Do not use beyond the specified number of tests.
- Warning, Product Contains Formamide. Formamide is toxic by inhalation and moderately toxic by ingestion. It is an irritant to skin, eyes, and mucous membranes and is absorbed through the skin. It may cause harm to the unborn child. Take precautions when handling reagents. Use disposable gloves and wear suitable protective clothing when handling suspected carcinogens or toxic materials.
- Materials of human or animal origin should be handled as potentially biohazardous and disposed of with proper precautions. In the event of exposure, the health directives of the responsible authorities should be followed.<sup>2,3</sup>
- Avoid contact of reagents with eyes, skin, and mucous membranes. If reagents come in contact with sensitive areas, wash with copious amounts of water. Avoid inhalation of reagents.
- Ensure that the waste container is empty prior to starting a run on the instrument. If this precaution is not taken, the waste container may overflow and the user risks a slip and fall.
- Avoid microbial contamination of reagents as this may produce incorrect results.
- For further information on the use of this device, refer to the BenchMark IHC/ISH instrument User Guide, and instructions for use of all necessary components located at [navifyportal.roche.com](http://navifyportal.roche.com).
- Consult local and/or state authorities to determine the recommended method of disposal.
- Product safety labeling primarily follows EU GHS guidance. Safety data sheet available for professional user on request.
- To report suspected serious incidents related to this device, contact the local Roche representative and the competent authority of the Member State or Country in which the user is established.

This product contains components classified as follows in accordance with the Regulation (EC) No. 1272/2008:

Table 1. Hazard Information

Hazard	Code	Statement
	H351	Suspected of causing cancer.
	H360D	May damage the unborn child.
	H373	May cause damage to organs through prolonged or repeated exposure.
	P201	Obtain special instructions before use.
	P202	Do not handle until all safety precautions have been read and understood.
	P260	Do not breathe mist or vapours.
	P280	Wear protective gloves/ protective clothing/ eye protection/ face protection/ hearing protection.
	P308 + P313	IF exposed or concerned: Get medical advice/ attention.

Hazard	Code	Statement
	P501	Dispose of contents/ container to an approved waste disposal plant.

This product contains CAS# 75-12-7: formamide

**STAINING PROCEDURE**

VENTANA probes have been developed for use on a BenchMark IHC/ISH instrument in combination with VENTANA detection kits and accessories. Recommended staining procedures and staining protocols for Alu Positive Control Probe on the BenchMark IHC/ISH instruments are listed in Table 2 and Table 3.

The parameters for the automated procedures can be displayed, printed and edited according to the procedure in the instrument User Guide. Refer to the appropriate VENTANA detection kit method sheet for more details.

For more details on the proper use of this device, refer to the inline dispenser method sheet (P/N 17377EN).

Table 2. Use the following staining procedures to perform Alu Positive Control Probe on BenchMark IHC/ISH instruments.

Instrument Platform	Staining Procedure
BenchMark GX	INFORM Alu Ctrl MIEWBlue V.1
BenchMark XT	XT INFORM Alu Ctrl MIEW Blue v3
BenchMark ULTRA and BenchMark ULTRA PLUS	U INFORM MIEW Blue ISH

Table 3. Recommended staining conditions for Alu Positive Control Probe on BenchMark IHC/ISH instruments.

Staining Condition	GX	XT	ULTRA or ULTRA PLUS <sup>a</sup>
Deparaffinization	Selected	Selected	Selected
Cell Conditioning Option	CC, Standard	CC, Standard	ULTRA CC2, Mild
ISH Protease 3	16 minutes	16 minutes	4 minutes
Probe	Alu Positive Control Probe	Alu Positive Control Probe	Alu Positive Control Probe
Counterstain	Red Counterstain II, 4 minutes	Red Counterstain II, 4 minutes	Red Counterstain II, 4 minutes

<sup>a</sup> Concordance was demonstrated between BenchMark ULTRA and BenchMark ULTRA PLUS instruments using representative assays.

Due to variation in tissue fixation and processing, as well as general lab instrument and environmental conditions, it may be necessary to increase or decrease the probe hybridization, cell conditioning or protease pretreatment based on individual specimens, detection used, and reader preference.

**QUALITY CONTROL PROCEDURES**

**Positive Specimen Control**

A laboratory-specific positive specimen control may be used with every staining procedure performed. Control specimens can be biopsy, surgical or fresh autopsy specimens prepared in a manner identical to patient specimens. Such controls are useful to monitor all steps of the procedure, from specimen preparation through staining. If a control specimen is prepared differently from the test specimens, then it will provide a control for the reagents, instrument and procedures, not for fixation and specimen processing. Results with the test specimens should be analyzed on the same run.

### Negative Specimen Control

A negative specimen control should be run with every staining procedure performed. The purpose is to monitor unintended probe and antibody cross reactivity to cellular components. The same specimen used for the positive specimen control may also be used as the negative specimen control. The variety of different cell types present in most specimens offers internal negative control sites, but this should be verified by the user. The non-staining components should demonstrate absence of specific staining and provide an indication of background staining. If unacceptable staining occurs in the negative specimen control sites, result with the patient specimens should be considered invalid.

### Negative Reagent Control

Negative reagent control should be substituted for the ISH probe with every specimen stained to aid in interpretation of each patient result. This provides an indication of nonspecific background staining for each slide. In place of the ISH probe, stain the slide with Negative Control Probe. The incubation period for controls should correspond to that of the probe.

The negative control is especially important with the finding that the intestinal form of alkaline phosphatase may be found in cells other than the brush border of intestinal epithelial cells. Additionally, enzymes capable of reducing nitro blue tetrazolium may be preserved during fixation.

### Unexplained Discrepancies

Unexplained discrepancies in controls should be referred to your local support representative immediately. If quality control results do not meet specifications, patient results are invalid. See the Troubleshooting section of this insert. Identify and correct the problem, then repeat the patient samples.

### Assay Verification

Prior to initial use of a reagent in a diagnostic procedure, the performance of the reagent should be verified by testing it on a series of positive and negative specimens with known ISH performance characteristics (refer to the Quality Control Procedures previously outlined in this section of the product insert, the Quality Control recommendations of the College of American Pathologists Laboratory Accreditation Program, Anatomic Pathology Checklist,<sup>4</sup> and the NCCLS Approved Guideline<sup>5</sup>). These quality control procedures should be repeated for each new lot of reagents, or whenever there is a change in assay parameters.

### STAINING INTERPRETATION / EXPECTED RESULTS

The VENTANA automated slide staining procedure causes a blue colored reaction product to precipitate at the target DNA sites localized by the labeled probe. A qualified pathologist experienced with the microscopic interpretation of anatomic pathology specimens, in ISH procedures, must evaluate positive and negative controls before interpreting results.

#### Controls

The stained positive control should be examined first to ascertain that all reagents are functioning properly. The presence of a blue colored reaction product within the target cells is indicative of positive reactivity.

The negative control should be examined after the positive control to verify the specificity of the reaction. There should be no specific staining in the negative control. If staining occurs, it may indicate non-specific cross reactivity to cells or cellular components. Intact cells should be used for interpretation of staining results since necrotic or degenerated cells often stain nonspecifically.

If the positive or negative control fails to demonstrate appropriate staining, any results with the test specimens should be considered invalid.

#### Patient Specimen

Patient specimens should be examined last. Positive staining intensity should be assessed within the context of any background staining of the negative reagent control. A negative result means that the DNA sequence in question was not detected, not necessarily that the sequence is absent in the cells assayed. The morphology of each sample should also be examined utilizing a hematoxylin and eosin stained section when interpreting any ISH result. The patient's morphologic findings and pertinent clinical data must be interpreted by a qualified pathologist.

### LIMITATIONS

#### General Limitations

1. ISH is a multiple step methodology that requires specialized training in the selection of the appropriate reagents, specimen preparation, processing, preparation of the ISH slide, and interpretation of the results.
2. Tissue staining is dependent on the handling and processing of the tissue prior to staining. Improper fixation, freezing, thawing, washing, drying, heating, sectioning, or contamination with other tissues or fluids may produce artifacts, antibody trapping, or false negative results. Inconsistent results may be a consequence of variations in fixation and embedding methods, or inherent irregularities within the tissue.
3. Excessive or incomplete counterstaining may compromise proper interpretation of results.
4. The clinical interpretation of staining must be evaluated within the context of clinical history, morphology, and other histopathological criteria. It is the responsibility of a qualified pathologist to be familiar with the reagents and methods used to produce the stained preparation. Staining must be performed in a certified, licensed laboratory under the supervision of a pathologist who is responsible for the review of the stained slides, and ensuring the adequacy of controls.
5. VENTANA reagents are provided at optimal dilution for use when the provided instructions are followed. Any deviation from recommended test procedures may invalidate expected results. Users must accept responsibility for interpretation of patient results when deviating from the recommended test procedures.
6. Due to variations in specimen processing it may be necessary to either increase or decrease the ISH protease treatment time or to use a different ISH protease on individual specimens. Such changes must be validated by the user. Users who deviate from recommended test procedures are responsible for interpretation of patient results under these circumstances.
7. Reagents may demonstrate unexpected reactions in previously untested tissues. The possibility of unexpected reactions even in tested tissue groups cannot be completely eliminated because of biological variability of tissues. Contact your local support representative with documented unexpected reactions.

#### Specific Limitations

1. When using fluorescein-labeled probes and the VENTANA ISH MIEW Blue Detection Kit, cytoplasmic and/or nuclear staining in epithelial cells of gastrointestinal tissue may be observed. Use of the Negative Control Probe is required to detect this staining.
2. All assays might not be registered on every instrument. Please contact your local support representative for more information.

### PERFORMANCE CHARACTERISTICS

#### ANALYTICAL PERFORMANCE

The performance of the Alu Positive Control Probe was evaluated through sensitivity, specificity, and precision studies. The following performance characteristics were demonstrated:

1. Sensitivity and specificity of Alu Positive Control Probe staining across a range of normal and neoplastic tissue types. Alu repeat DNA sequence was detected in the nuclei of cells in the majority of tissue types, and tumors, with a lack of significant background or cross-reactivity.
2. Specificity of Alu Positive Control Probe by the presence of signal on normal (untreated) human spleen tissue and the absence of signal on DNase1 treated human spleen tissue.
3. Between lot precision of the probe.
4. Within run and between day precision on a BenchMark ULTRA instrument.
5. Between instrument precision on a BenchMark GX, BenchMark XT, and BenchMark ULTRA instrument.
6. Between platform precision between the BenchMark GX, BenchMark XT, and BenchMark ULTRA instrument.

All studies met their acceptance criteria.

Precision on the BenchMark ULTRA PLUS instrument was demonstrated using representative assays. Studies included Within-run Repeatability, Between-day and Between-run Intermediate Precision. All studies met their acceptance criteria.

## TROUBLESHOOTING

Table 1. Troubleshooting solutions.

Issue	Solution
Positive control is negative.	Check that the slide has the proper barcode label.
Positive control is negative or exhibits weaker staining than expected.	Check other positive controls stained on the same staining run to determine if the failure is due to the control slide or reagents used. Positive control specimens are recommended for potential troubleshooting for each run.
Tissue washes off slides.	Ensure that positively-charged slides are used.
Sections thicker than 4 µm exhibit nuclear bubbling due to excess paraffin.	Select the "extended deparaffinization" option in the staining procedure.

## REFERENCES

1. Carson FL, Cappellano C. *Histotechnology; A Self-Instructional Text*, 5th edition. American Society for Clinical Pathology Press; 2020, 2022.
2. Occupational Safety and Health Standards: Occupational exposure to hazardous chemicals in laboratories. (29 CFR Part 1910.1450). Fed. Register.
3. Directive 2000/54/EC of the European Parliament and Council of 24 June 2020 on the protection of workers from risks related to exposure to biological agents at work.
4. College of American Pathologists Laboratory Accreditation Program, Anatomic Pathology Checklist, 2001.
5. NCCLS. *Quality Assurance for Immunocytochemistry: Approved Guideline*. NCCLS document MM4-A- (ISBN 1-56238-396-5). NCCLS, 940 West Valley Road, Suite 1400, Wayne, PA 19087-1898 USA, 1999.

NOTE: A point (period/stop) is always used in this document as the decimal separator to mark the border between the integral and the fractional parts of a decimal numeral. Separators for thousands are not used.

## Symbols

Ventana uses the following symbols and signs in addition to those listed in the ISO 15223-1 standard (for USA: see [elabdoc.roche.com/symbols](http://elabdoc.roche.com/symbols) for more information).

**GTIN** Global Trade Item Number

Rx only For USA: Caution: Federal law restricts this device to sale by or on the order of a physician.

## REVISION HISTORY

Rev	Updates
H	Correction to Table 2 in the Staining Procedure section. Updated to current template.

## INTELLECTUAL PROPERTY

VENTANA, BENCHMARK, and INFORM are trademarks of Roche. All other product names and trademarks are the property of their respective owners.

© 2025 Ventana Medical Systems, Inc.

For USA: Rx only

## CONTACT INFORMATION



Ventana Medical Systems, Inc.  
1910 E. Innovation Park Drive  
Tucson, AZ 85755  
USA  
+1 520 887 2155  
+1 800 227 2155 (USA)

[www.roche.com](http://www.roche.com)



Roche Diagnostics GmbH  
Sandhofer Strasse 116  
68305 Mannheim  
Germany  
+800 5505 6606

