

cobas[®]



Rx Only

cobas[®] **EGFR Mutation Test v2**

For in vitro diagnostic use



cobas[®] **EGFR Mutation Test v2**

24 Tests P/N: 07248563190

For FFPET samples, refer to the **cobas**[®] DNA Sample Preparation Kit (M/N 05985536190) for sample preparation.

For plasma samples, refer to the **cobas**[®] cfDNA Sample Preparation Kit (M/N 07247737190) for sample preparation.

TABLE OF CONTENTS

Intended use

Summary and explanation of the test

Background	7
Principles of the procedure	9
Sample preparation	9
PCR amplification	9

SECTION A: FOR USE WITH TISSUE SAMPLES

Materials and reagents

Materials and reagents provided	11
Reagent storage and handling	12
Additional materials required	13
Instrumentation and software required but not provided	13

Precautions and handling requirements

Warnings and precautions	13
Good laboratory practice	14
Contamination	14
Integrity	14
Disposal	14
Spillage and cleaning	15

Sample collection, transport, and storage

Sample collection	15
Sample transport, storage, and stability	15
Processed sample storage and stability	15

Test procedure

Running the test	16
Instructions for use	16
Run size	16
Full process control	16
DNA isolation	16
Macro-dissection	17
DNA quantitation	17
Amplification and detection	17
Instrument set-up	17
Test order set-up	18
Dilution calculation of sample DNA stock	19
Sample dilution	19
Reaction set-up	20
Starting PCR	21

Results

Interpretation of results.....	22
Retesting of samples with invalid results	22
Quality control and validity of results	23
Mutant control.....	23
Negative control	23
Procedural limitations	23

Non-clinical performance evaluation

Analytical sensitivity – limit of blank.....	24
Limit of detection using FFPET specimen blends	24
Minimal tumor content.....	26
Cross-reactivity to other exon 18, 19, 20, and 21 mutations.....	27
EURTAC clinical trial specimens	27
AURA2 clinical trial specimens	27
Specificity – microorganisms and EGFR homologs.....	27
Lung-related microorganisms	27
Plasmids of EGFR homologs	27
Interference	28
Necrotic tissue.....	28
Repeatability.....	28
Specimen handling reproducibility	28

Clinical performance evaluation

Clinical reproducibility study 1	29
Clinical reproducibility study 2	30
Correlation to reference method using Phase III samples from EURTAC trial	31
Correlation to reference method using Phase II samples from AURA2	33
Clinical outcome data	34
EURTAC.....	34
AURA2.....	35
FLAURA.....	36

SECTION B: FOR USE WITH PLASMA SAMPLES**Sample preparation****Materials and reagents**

Materials and reagents provided	40
Reagent storage and handling.....	41
Additional materials required	42
Instrumentation and software required but not provided	42

Precautions and handling requirements

Warnings and precautions.....	42
-------------------------------	----

Good laboratory practice.....	43
Contamination.....	43
Integrity	43
Disposal	43
Spillage and cleaning.....	44
Sample collection, transport, and storage	
Sample collection and handling	44
Sample transport, storage and stability	44
Processed sample storage and stability.....	45
Test procedure	
Running the test.....	46
Instructions for use	46
Run size.....	46
Full process control.....	46
DNA isolation	46
Amplification and detection	47
Instrument set-up.....	47
Test order set-up	47
Reaction set-up	48
Starting PCR.....	49
Results	
Interpretation of results.....	50
Semi Quantitative Index (SQI).....	50
Retesting of samples with invalid results	51
Quality control and validity of results	51
Mutant control.....	51
Negative control	51
Procedural limitations	51
Non-clinical performance evaluation	
Analytical performance	53
Analytical sensitivity – limit of blank.....	53
Limit of detection using cell line DNA.....	53
Cross reactivity to other Exon 18, 19, 20, and 21 mutations.....	54
AURA Extension and AURA2 clinical trial samples.....	54
Specificity – microorganism	54
Interference	54
Linearity.....	55
Repeatability.....	58

Clinical performance evaluation

Clinical reproducibility with K2 EDTA plasma.....	59
Clinical reproducibility with Roche cfDNA plasma.....	60
Limit of Detection (LOD) using NSCLC plasma samples.....	61
Correlation of Roche cfDNA plasma to K2 EDTA plasma.....	62
Correlation to reference method using Phase III plasma samples from the ASPIRATION cohort.....	63
Correlation between plasma and tissue samples by the cobas EGFR Test for the detection of exon 19 deletion and L858R mutations using Phase III samples from ENSURE.....	64
Correlation to reference method using Phase II samples from AURA2.....	65
Correlation between plasma and tissue samples for the detection of T790M using Phase II samples from AURA2.....	66
Clinical outcome data.....	67
ENSURE.....	67
AURA2.....	69
FLAURA.....	69

Result flags

Explanation of result flags.....	73
----------------------------------	----

Additional information

Symbols.....	75
Technical support.....	76
Manufacturer.....	76
Trademarks and patents.....	76
Copyright.....	76
References.....	77
Document revision.....	79

Intended use

The **cobas**® EGFR Mutation Test v2 is a real-time PCR test for the qualitative detection of defined mutations of the epidermal growth factor receptor (EGFR) gene in non-small cell lung cancer (NSCLC) patients. Defined EGFR mutations are detected using DNA isolated from formalin-fixed paraffin-embedded tumor tissue (FFPET) or circulating-free tumor DNA (cfDNA) from plasma derived from EDTA anti-coagulated peripheral whole blood.

The test is indicated as a companion diagnostic to aid in selecting NSCLC patients for treatment with EGFR tyrosine kinase inhibitors (including the targeted therapies listed in Table 1 below) in accordance with the approved therapeutic product labeling:

Table 1

Drug	FFPET	Plasma
TARCEVA® (erlotinib)	Exon 19 deletions and L858R	Exon 19 deletions and L858R
TAGRISSO® (osimertinib)	Exon 19 deletions, L858R and T790M	Exon 19 deletions, L858R and T790M
IRESSA® (gefitinib)	Exon 19 deletions and L858R	Exon 19 deletions and L858R

Testing of plasma specimens is most appropriate for consideration in patients from whom a tumor biopsy cannot be obtained. Patients who are negative for these mutations by this test using plasma specimens should be reflexed to routine tissue biopsy and testing for EGFR mutations with the FFPET sample type, if available.

Drug safety and efficacy have not been established for the following EGFR mutations also detected by the **cobas**® EGFR Mutation Test v2:

Table 2

Drug	FFPET	Plasma
TARCEVA® (erlotinib)	G719X, Exon 20 insertions, T790M, S768I and L861Q	G719X, Exon 20 insertions, T790M, S768I and L861Q
TAGRISSO® (osimertinib)	G719X, Exon 20 insertions, S768I, and L861Q	G719X, Exon 20 insertions, S768I, and L861Q
IRESSA® (gefitinib)	G719X, Exon 20 insertions, T790M, S768I and L861Q	G719X, Exon 20 insertions, T790M, S768I and L861Q

The **cobas**® EGFR Mutation Test v2 for use with plasma includes a semi-quantitative measurement of mutations in exons 18, 19, 20, and 21 of the EGFR gene. This measurement, reported as a semi-quantitative index (SQI), correlates to the amount of target mutant cfDNA in plasma and can be used to determine changes in target mutant cfDNA load over time for a given patient.

For manual sample preparation, FFPET specimens are processed using the **cobas**® DNA Sample Preparation Kit and plasma specimens are processed using the **cobas**® cfDNA Sample Preparation Kit. The **cobas**® z 480 analyzer is used for automated amplification and detection.

Summary and explanation of the test

Background

Activating mutations in the gene encoding EGFR occur primarily in NSCLC, and result in constitutive activation of the kinase activity of the EGFR protein, thereby contributing to the oncogenic process.¹ The prevalence of these mutations in unselected cases of NSCLC is approximately 10% - 30%.^{2,3} However, these mutations occur more frequently, but not exclusively, in non-smoking/light-smoking female patients of Asian ancestry with adenocarcinoma histologies.⁴

The most common EGFR mutations in NSCLC include a variety of deletions in exon 19 and the substitution mutation L858R in exon 21; these mutations collectively constitute approximately 85% of EGFR mutations observed in NSCLC.⁵ The **cobas**® EGFR Mutation Test v2 (**cobas** EGFR Test) is a real-time PCR assay designed to detect G719X substitution mutations in exon 18, deletion mutations in exon 19, T790M and S768I substitution mutations in exon 20, insertion mutations in exon 20, and L858R and L861Q substitution mutations in exon 21.

The **cobas** EGFR Test is used as a companion diagnostic test for TARCEVA® (erlotinib), a compound that reversibly inhibits the kinase activity of EGFR, preventing autophosphorylation of tyrosine residues associated with the receptor and thereby inhibiting further downstream signaling that promotes cell survival and proliferation. TARCEVA® binding affinity for EGFR exon 19 deletion or exon 21 L858R mutations is higher than its affinity for the wild-type receptor.⁶ Clinical trials have shown that patients with advanced NSCLC and with exon 19 deletion mutations or exon 21 L858R substitution mutations that were treated with TARCEVA® as first-line treatment, are likely to experience clinical benefit compared to patients treated with chemotherapy.^{3,7}

The **cobas** EGFR Test is used as a companion diagnostic test for TAGRISSO® (osimertinib), an irreversible inhibitor of both EGFR TKI-sensitizing and T790M resistance mutations in advanced NSCLC. TAGRISSO® inhibits the kinase activity of EGFR, which inhibits a cascade of intracellular downstream signaling events that promote cell proliferation, survival, and angiogenesis.⁸ Clinical trials have shown that patients with advanced non-squamous NSCLC with an EGFR TKI-sensitizing mutation and have progressed following therapy with a first generation EGFR TKI and who have developed a T790M resistance mutation in exon 20 that were treated with TAGRISSO® are likely to experience clinical benefit.⁹ A phase III clinical trial demonstrated that patients with advanced NSCLC (exon 19 deletion or exon 21 L858R substitution mutation positive) that were treated with TAGRISSO® as first-line treatment, had greater clinical benefit compared to patients treated with a first generation EGFR TKI (gefitinib or erlotinib).¹⁰

The **cobas** EGFR Test is used as a companion diagnostic test for IRESSA® (gefitinib), a compound that reversibly inhibits the kinase activity of EGFR, preventing autophosphorylation of tyrosine residues associated with the receptor and thereby inhibiting further downstream signaling that promotes cell survival and proliferation. Clinical trials have shown that patients with advanced NSCLC and with exon 19 deletion mutations or exon 21 L858R substitution mutations that were treated with IRESSA® as first-line treatment, are likely to experience clinical benefit compared to patients treated with chemotherapy.^{11,12,13}

Table 3 lists the EGFR mutations detected by the **cobas** EGFR Test.

Table 3 The cobas EGFR Test is designed to detect the following mutations

Exon	EGFR Mutation Group	EGFR Nucleic Acid Sequence	HGVS* Protein Nomenclature	HGVS* Nucleotide Nomenclature	COSMIC ID ¹⁴
Exon 18	G719X	2156G>C	LRG_304p1:p.(Gly719Ala)	LRG_304t1:c.2156G>C	6239
		2155G>A	LRG_304p1:p.(Gly719Ser)	LRG_304t1:c.2155G>A	6252
		2155G>T	LRG_304p1:p.(Gly719Cys)	LRG_304t1:c.2155G>T	6253
Exon 19	Ex19Del	2240_2251del12	LRG_304p1:p.(Leu747_Thr751delinsSer)	LRG_304t1:c.2240_2251delTAAGAGAAGCAA	6210
		2239_2247del9	LRG_304p1:p.(Leu747_Glu749del)	LRG_304t1:c.2239_2247delTTAAGAGAA	6218
		2238_2255del18	LRG_304p1:p.(Glu746_Ser752delinsAsp)	LRG_304t1:c.2238_2255delATTAAGAGAAGCAACATC	6220
		2235_2249del15	LRG_304p1:p.(Glu746_Ala750del)	LRG_304t1:c.2235_2249delGGAATTAAGAGAAGC	6223
		2236_2250del15	LRG_304p1:p.(Glu746_Ala750del)	LRG_304t1:c.2236_2250delGAATTAAGAGAAGCA	6225
		2239_2253del15	LRG_304p1:p.(Leu747_Thr751del)	LRG_304t1:c.2240_2254delTAAGAGAAGCAACAT	6254
		2239_2256del18	LRG_304p1:p.(Leu747_Ser752del)	LRG_304t1:c.2239_2256delTTAAGAGAAGCAACA TCT	6255
		2237_2254del18	LRG_304p1:p.(Glu746_Ser752delinsAla)	LRG_304t1:c.2237_2254delAATTAAGAGAAGCAACAT	12367
		2240_2254del15	LRG_304p1:p.(Leu747_Thr751del)	LRG_304t1:c.2240_2254delTAAGAGAAGCAACAT	12369
		2240_2257del18	LRG_304p1:p.(Leu747_Pro753delinsSer)	LRG_304t1:c.2240_2257delTAAGAGAAGCAACATCTC	12370
		2239_2248TTAAGAGAAG>C	LRG_304p1:p.(Leu747_Ala750delinsPro)	LRG_304t1:c.2239_2248delinsC	12382
		2239_2251>C	LRG_304p1:p.(Leu747_Thr751delinsPro)	LRG_304t1:c.2239_2251delinsC	12383
		2237_2255>T	LRG_304p1:p.(Glu746_Ser752delinsVal)	LRG_304t1:c.2237_2255delinsT	12384
		2235_2255>AAT	LRG_304p1:p.(Glu746_Ser752delinsIle)	LRG_304t1:c.2235_2255delinsAAT	12385
		2237_2252>T	LRG_304p1:p.(Glu746_Thr751delinsVal)	LRG_304t1:c.2237_2252delinsT	12386
		2239_2258>CA	LRG_304p1:p.(Leu747_Pro753delinsGln)	LRG_304t1:c.2239_2258delinsCA	12387
		2239_2256>CAA	LRG_304p1:p.(Leu747_Ser752delinsGln)	LRG_304t1:c.2239_2256delinsCAA	12403
		2237_2253>TTGCT	LRG_304p1:p.(Glu746_Thr751delinsValAla)	LRG_304t1:c.2237_2253delinsTTGCT	12416
		2238_2252>GCA	LRG_304p1:p.(Leu747_Thr751delinsGln)	LRG_304t1:c.2238_2252delinsGCA	12419
		2238_2248>GC	LRG_304p1:p.(Leu747_Ala750delinsPro)	LRG_304t1:c.2238_2248delinsGC	12422
		2237_2251del15	LRG_304p1:p.(Glu746_Thr751delinsAla)	LRG_304t1:c.2237_2251delAATTAAGAGAAGCAA	12678
		2236_2253del18	LRG_304p1:p.(Glu746_Thr751del)	LRG_304t1:c.2236_2253delGAATTAAGAGAAGCAACA	12728
		2235_2248>AATTC	LRG_304p1:p.(Glu746_Ala750delinsIlePro)	LRG_304t1:c.2235_2248delinsAATTC	13550
		2235_2252>AAT	LRG_304p1:p.(Glu746_Thr751delinsIle)	LRG_304t1:c.2235_2252delinsAAT	13551
		2235_2251>AATTC	LRG_304p1:p.(Glu746_Thr751delinsIlePro)	LRG_304t1:c.2235_2251delinsAATTC	13552
		2253_2276del24	LRG_304p1:p.(Ser752_Ile759del)	LRG_304t1:c.2253_2276delATCTCCGAAAGCCAA CAAGGAAAT	13556
		2237_2257>TCT	LRG_304p1:p.(Glu746_Pro753delinsValSer)	LRG_304t1:c.2237_2257delinsTCT	18427
		2238_2252del15	LRG_304p1:p.(Leu747_Thr751del)	LRG_304t1:c.2240_2254delTAAGAGAAGCAACAT	23571
2233_2247del15	LRG_304p1:p.(Lys745_Glu749del)	LRG_304t1:c.2233_2247delAAGGAATTAAGAGAA	26038		
Exon 20	S768I	2303G>T	LRG_304p1:p.(Ser768Ile)	LRG_304t1:c.2303G>T	6241
	T790M	2369C>T	LRG_304p1:p.(Thr790Met)	LRG_304t1:c.2369C>T	6240
	Ex20Ins	2307_2308ins9GCCAGCGTG	LRG_304p1:p.(Ala767_Val769dup)	LRG_304t1:c.2300_2308dupCCAGCGTGG	12376
		2319_2320insCAC	LRG_304p1:p.(His773dup)	LRG_304t1:c.2317_2319dupCAC	12377
		2310_2311insGGT	LRG_304p1:p.(Asp770_Asn771insGly)	LRG_304t1:c.2310_2311insGGT	12378
2311_2312ins9GCGTGGACA		LRG_304p1:p.(Ser768_Asp770dup)	LRG_304t1:c.2303_2311dupGCGTGGACA	13428	
	2309_2310AC>CCAGCGTGGAT	LRG_304p1:p.(Ala767_Val769dup)	LRG_304t1:c.2309_2310delinsCCAGCGTGGAT	13558	
Exon 21	L858R	2573T>G	LRG_304p1:p.(Leu858Arg)	LRG_304t1:c.2573T>G	6224
		2573_2574TG>GT	LRG_304p1:p.(Leu858Arg)	LRG_304t1:c.2573_2574delinsGT	12429
	L861Q	2582T>A	LRG_304p1:p.(Leu861Gln)	LRG_304t1:c.2582T>A	6213

* HGVS – Human Genome Variation Society

Principles of the procedure

The **cobas** EGFR Test is based on two major processes: (1) manual sample preparation to obtain DNA from FFPE or plasma; and (2) PCR amplification and detection of target DNA using complementary primer pairs and oligonucleotide probes labeled with fluorescent dyes. The **cobas** EGFR Test is designed to detect the following mutations:

- Exon 18: G719X (G719A, G719C, and G719S)
- Exon 19: deletions and complex mutations (defined as the combination of a deletion and an insertion)
- Exon 20: S768I, T790M, and insertions
- Exon 21: L858R and L861Q

Mutation detection is achieved through PCR analysis with the **cobas**® z 480 analyzer. A mutant control and negative control are included in each run to confirm the validity of the run.

Sample preparation

The **cobas**® DNA Sample Preparation Kit and the **cobas**® cfDNA Sample Preparation Kit are for manual sample preparations from FFPE and plasma respectively, based on nucleic acid binding to glass fibers. A protease and chaotropic lysis/binding buffer releases nucleic acids and protects the released DNA from DNases. Subsequently, isopropanol is added to the lysis mixture that is then centrifuged through a column with a glass fiber filter insert. During centrifugation, the DNA is bound to the surface of the glass fiber filter. Unbound substances, such as salts, proteins and other cellular impurities, are removed by centrifugation. The adsorbed nucleic acids are washed and then eluted with an aqueous solution. The target DNA is then amplified and detected on the **cobas**® z 480 analyzer using the amplification and detection reagents provided in the **cobas** EGFR Test kit.

PCR amplification

Target selection

The **cobas** EGFR Test uses primers that define specific base-pair sequences for each of the targeted mutations. For the exon 19 deletion mutations, sequences ranging from 125 to 141 base pairs are targeted; for the L858R substitution mutation in exon 21, a 138 base pair sequence is targeted; for the T790M substitution mutation in exon 20, a 118 base pair sequence is targeted; for the G719X substitution mutation in exon 18, sequences ranging from 104-106 base pairs are targeted; for the S768I substitution mutation in exon 20, a 133 base pair sequence is targeted; for the exon 20 insertion mutations, sequences ranging from 125 to 143 base pairs are targeted; for the L861Q substitution mutation in exon 21, a 129 base pair sequence is targeted. Amplification occurs only in the regions of the EGFR gene between the primers; the entire EGFR gene is not amplified.

Target amplification

A derivative of *Thermus* species Z05-AS1 DNA polymerase is utilized for target amplification. First, the PCR mixture is heated to denature the DNA and expose the primer target sequences. As the mixture cools, the upstream and downstream primers anneal to the target DNA sequences. The Z05 DNA polymerase, in the presence of divalent metal cation and excess dNTP, extends each annealed primer, thus synthesizing a second DNA strand. This completes the first cycle of PCR, yielding a double-stranded DNA copy which includes the targeted base-pair regions of the EGFR gene. This process is repeated for a number of cycles, with each cycle effectively doubling the amount of amplicon DNA.

Automated real-time mutation detection

The **cobas** EGFR Test utilizes real-time PCR technology. Each target-specific, oligonucleotide probe in the reaction is labeled with a fluorescent dye that serves as a reporter, and with a quencher molecule that absorbs (quenches) fluorescent emissions from the reporter dye within an intact probe. During each cycle of amplification, the probe complementary to the single-stranded DNA sequence in the amplicon binds and is subsequently cleaved by the 5' to 3' nuclease activity of the Z05-AS1 DNA Polymerase. Once the reporter dye is separated from the quencher by this nuclease activity, fluorescence of a characteristic wavelength can be measured when the reporter dye is excited by the appropriate spectrum of light. Four different reporter dyes are used to label the mutations targeted by the test. Amplification of the seven targeted EGFR sequences are detected independently across three reactions by measuring fluorescence at the four characteristic wavelengths in dedicated optical channels.

Selective amplification

Selective amplification of target nucleic acid from the sample is achieved in the **cobas** EGFR Test by the use of AmpErase (uracil-N-glycosylase) enzyme and deoxyuridine triphosphate (dUTP).¹⁵ The AmpErase enzyme recognizes and catalyzes the destruction of DNA strands containing deoxyuridine but not DNA containing thymidine. Deoxyuridine is not present in naturally occurring DNA but is always present in amplicon due to the use of dUTP in place of deoxythymidine triphosphate as one of the nucleotide triphosphates in the Master Mix reagents; therefore, only amplicon contains deoxyuridine. Deoxyuridine renders contaminating amplicon susceptible to destruction by AmpErase enzyme prior to amplification of the target DNA. The AmpErase enzyme, which is included in the Master Mix reagents, catalyzes the cleavage of deoxyuridine-containing DNA at the deoxyuridine residues by opening the deoxyribose chain at the C1-position. When heated in the first thermal cycling step at alkaline pH, the amplicon DNA chain breaks at the position of the deoxyuridine, thereby rendering the DNA non-amplifiable. The AmpErase enzyme is inactive at temperatures above 55°C, i.e., throughout the thermal cycling steps, and therefore does not destroy target amplicon. The **cobas** EGFR Test has been demonstrated to inactivate deoxyuridine-containing EGFR mutant amplicon.

FOLLOW INSTRUCTIONS IN SECTION A FOR USE WITH TISSUE SAMPLES.
FOLLOW INSTRUCTIONS IN SECTION B FOR USE WITH PLASMA SAMPLES.

SECTION A: FOR USE WITH TISSUE SAMPLES

Refer to the cobas® DNA Sample Preparation Kit (M/N 05985536190) for the isolation of DNA from tissue samples.

Materials and reagents

Materials and reagents provided

Kit/Cassettes	Components and Reagent Ingredients	Quantity per Test	Safety Symbol and Warning
cobas® EGFR Mutation Test v2 24 Tests (M/N: 07248563190)	EGFR MMX-1 (EGFR Master Mix 1) (M/N 06471366001) Tris buffer Potassium chloride Glycerol EDTA Tween 20 3.13% Dimethyl sulfoxide 0.09% Sodium azide < 0.10% dNTPs < 0.01% Z05-AS1 DNA polymerase (microbial) <0.01% AmpErase (uracil-N-glycosylase) enzyme (microbial) < 0.01% Aptamer < 0.01% Upstream and downstream EGFR primers < 0.01% Fluorescent labeled EGFR probes	2 x 0.48 mL	N/A
	EGFR MMX-2 (EGFR Master Mix 2) (M/N 06471382001) Tris buffer Potassium chloride Glycerol EDTA Tween 20 3.13% Dimethyl sulfoxide 0.09% Sodium azide <0.10% dNTPs < 0.01% Z05-AS1 DNA polymerase (microbial) < 0.01% AmpErase (uracil-N-glycosylase) enzyme (microbial) < 0.01% Aptamer < 0.01% Upstream and downstream EGFR primers < 0.01% Fluorescent labeled EGFR probes	2 x 0.48 mL	N/A

Kit/Cassettes	Components and Reagent Ingredients	Quantity per Test	Safety Symbol and Warning
cobas® EGFR Mutation Test v2 24 Tests (M/N: 07248563190)	EGFR MMX-3 v2 (EGFR Master Mix 3) (M/N 07248610001) Tris buffer Potassium chloride Glycerol EDTA Tween 20 3.13% Dimethyl sulfoxide 0.09% Sodium azide < 0.10% dNTPs < 0.01% Z05-AS1 DNA polymerase (microbial) < 0.01% AmpErase (uracil-N-glycosylase) enzyme (microbial) < 0.01% Aptamer < 0.01% Upstream and downstream EGFR primers < 0.01% Fluorescent labeled EGFR probes	2 x 0.48 mL	N/A
	MGAC (Magnesium acetate) (M/N 05854326001) Magnesium acetate 0.09% Sodium azide	6 x 0.2 mL	N/A
	EGFR MC (EGFR Mutant Control) (M/N 06471455001) Tris buffer EDTA Poly-rA RNA (synthetic) 0.05% Sodium azide < 0.1% Plasmid DNA containing EGFR exon 18, 19, 20 and 21 sequences (microbial) < 0.1% EGFR wild-type DNA (cell culture)	6 x 0.1 mL	N/A
	DNA SD (DNA Specimen Diluent) (M/N 05854474001) Tris-HCl buffer 0.09% Sodium azide	2 x 3.5 mL	N/A

Reagent storage and handling

Reagent	Storage Temperature	Storage Time
cobas® EGFR Mutation Test v2*	2°C to 8°C	Once opened, stable for 4 uses over 90 days or until the expiration date indicated, whichever comes first.

* **EGFR MMX-1, EGFR MMX-2, EGFR MMX-3 v2**, and working MMX (prepared by the addition of **MGAC** to **EGFR MMX-1** or **EGFR MMX-2** or **EGFR MMX-3 v2**) should be protected from prolonged exposure to light. Working MMX must be stored at 2°C to 8°C in the dark. The prepared samples and controls must be added within 1 hour of preparation of the working MMX. Amplification must be started within 1 hour from the time that the processed samples and controls are added to the working MMX.

Additional materials required

Materials	M/N
cobas® DNA Sample Preparation Kit	Roche 05985536190
Bleach	Any vendor
70% Ethanol	Any vendor
cobas® 4800 System Microwell Plate (AD-plate) and sealing film	Roche 05232724001
cobas® 4800 System sealing film applicator (supplied with the installation of the cobas® 4800 System)	Roche 04900383001
Adjustable pipettors* (Capable of pipetting 5 - 1000 µL)	Any vendor
Aerosol barrier or positive displacement DNase-free tips	Any vendor
Locking-lid microcentrifuge tubes (1.5 mL sterile, RNase/DNase free, PCR grade)	Any vendor
Microcentrifuge tube racks	Any vendor
Spectrophotometer for measuring DNA concentration*	Any vendor
Vortex mixer*	Any vendor
Disposable gloves, powder-free	Any vendor
Freezer capable of -25°C to -15°C storage	Any vendor

* All equipment should be maintained according to the manufacturer's instructions.

For more information regarding the materials sold separately, contact your local Roche representative.

Instrumentation and software required but not provided

Required Instrumentation and Software, Not Provided
cobas® z 480 Analyzer
cobas® 4800 System Control Unit with System Software version 2.2 or higher
EGFR Tissue P1 Analysis Package Software version 1.0 or higher*
Barcode Reader ext USB
Printer

* Refer to the cobas® EGFR Mutation Test v2 kit's Product Information Card (M/N: 07335873001) for the current software version.

For more information regarding the materials sold separately, contact your local Roche representative.

Precautions and handling requirements

Warnings and precautions

As with any test procedure, good laboratory practice is essential to the proper performance of this assay.

- For in vitro diagnostic use only.
- Safety Data Sheets (SDS) are available upon request from your local Roche office.
- This test is for use with FFPET NSCLC samples. Samples should be handled as if infectious using safe laboratory procedures such as those outlined in Biosafety in Microbiological and Biomedical Laboratories¹⁶ and in the CLSI Document M29-A4.¹⁷
- The use of sterile disposable pipettes and DNase-free pipettor tips is recommended.

Good laboratory practice

- Do not pipette by mouth.
- Do not eat, drink or smoke in laboratory work areas.
- Wash hands thoroughly after handling samples and kit reagents.
- Wear eye protection, laboratory coats and disposable gloves when handling any reagents. Avoid contact of these materials with the skin, eyes or mucous membranes. If contact does occur, immediately wash with large amounts of water. Burns can occur if left untreated. If spills occur, dilute with water before wiping dry.
- Thoroughly clean and disinfect all laboratory work surfaces with a freshly prepared solution of 0.5% sodium hypochlorite in distilled or deionized water (dilute household bleach 1:10). Follow by wiping the surface with 70% ethanol.

Note: *Commercial liquid household bleach typically contains sodium hypochlorite at a concentration of 5.25%. A 1:10 dilution of household bleach will produce a 0.5% sodium hypochlorite solution.*

Contamination

- Gloves must be worn and must be changed between handling samples and **cobas** EGFR Test reagents to prevent contamination. Avoid contaminating gloves when handling samples.
- Gloves must be changed frequently to reduce the potential for contamination.
- Gloves must be changed before leaving DNA Isolation areas or if contact with solutions or a sample is suspected.
- Avoid microbial and ribonuclease contamination of reagents.
- The amplification and detection work area should be thoroughly cleaned before working MMX preparation. Supplies and equipment should be dedicated to each activity and not used for other activities or moved between areas. For example, pipettors and supplies used for DNA Isolation must not be used to prepare reagents for amplification and detection.
- It is highly recommended that workflow in the laboratory proceed in a uni-directional manner, completing one activity before proceeding to the next activity. For example, DNA isolation should be completed before starting amplification and detection. DNA isolation should be performed in an area separate from amplification and detection. To avoid contamination of the working master mix with DNA samples, the amplification and detection work area should be thoroughly cleaned before working master mix preparation.

Integrity

- Do not use kits after their expiration dates.
- Do not pool reagents from different kits or lots.
- Do not use disposable items beyond their expiration date.
- All disposable items are for one time use. Do not reuse.
- All equipment should be properly maintained according to the manufacturer's instructions.

Disposal

- **MGAC, EGFR MMX-1, EGFR MMX-2, EGFR MMX-3 v2, EGFR MC, and DNA SD** contain sodium azide. Sodium azide may react with lead and copper plumbing to form highly explosive metal azides. While disposing of sodium azide containing solutions down laboratory sinks, flush the drains with a large volume of cold water to prevent azide buildup.
- Dispose of unused reagents and waste in accordance with country, federal, state and local regulations.

Spillage and cleaning

- If spills occur on the cobas® 4800 instrument, follow the instructions in the appropriate cobas® 4800 System – Operator’s Manual or cobas® 4800 System – User Assistance to clean.
- Do not use sodium hypochlorite solution (bleach) for cleaning the cobas® z 480 analyzer. Clean the cobas® z 480 analyzer according to procedures described in the appropriate cobas® 4800 System – Operator’s Manual or cobas® 4800 System - User Assistance.
- For additional warnings, precautions and procedures to reduce the risk of contamination for the cobas® z 480 analyzer, consult the cobas® 4800 System – Operator’s Manual or cobas® 4800 System - User Assistance.

Sample collection, transport, and storage

Note: Handle all samples as if they are capable of transmitting infectious agents.

Sample collection

NSCLC FFPET samples have been validated for use with the cobas EGFR Test.

Sample transport, storage, and stability

NSCLC FFPET samples can be transported at 15°C to 30°C. Transportation of FFPET samples must comply with country, federal, state, and local regulations for the transport of etiologic agents.¹⁸

Stability of FFPET samples has been verified for up to 12 months after the date of collection, when stored at 15°C to 30°C. Five-µm sections mounted on slides may be stored at 15°C to 30°C for up to 60 days.

FFPET samples are stable for either:

FFPET Sample Type	FFPET Block	5 µm FFPET Section
FFPET Sample Storage Temperature	15°C to 30°C	15°C to 30°C
Storage Time	Up to 12 months	Up to 60 days

Processed sample storage and stability

Processed samples (extracted DNA) are stable at one of the following:

Extracted DNA Storage Temperature	-15°C to -25°C	2°C to 8°C	15°C to 30°C
Storage Time	Up to 3 freeze thaws over 60 days	Up to 14 days	Up to 1 day

Extracted DNA should be used within the recommended storage periods or before the expiration date of the cobas® DNA Sample Preparation Kit used to extract the DNA, whichever comes first.

Test procedure

Running the test

Figure 1 cobas EGFR Test workflow with cobas® DNA Sample Preparation Kit

1	Start the system
2	Perform instrument maintenance
3	Remove samples and reagents from storage
4	Deparaffinize samples
5	Perform DNA isolation
6	Elute DNA
7	Create work order and print plate layout
8	Prepare amplification reagents
9	Load AD-plate with amplification reagents
10	Load AD-plate with sample
11	Seal AD-plate
12	Load AD-plate on the cobas® z 480 analyzer
13	Start the run
14	Review results
15	With LIS: send results to LIS
16	Unload analyzer

Instructions for use

Note: Only NSCLC FFPET sections of 5- μ m thickness containing at least 10% tumor content by area are to be used in the cobas EGFR Test. Any sample containing less than 10% tumor content by area should be macro-dissected after deparaffinization.

Note: Refer to the cobas® 4800 System – Operator’s Manual or cobas® 4800 System - User Assistance for detailed operating instructions for the cobas® z 480 analyzer.

Run size

A single run can include from 1 to 30 samples (plus controls) per 96-well microwell plate. When running more than 24 samples, multiple cobas EGFR Test kits will be required.

The cobas EGFR Test contains sufficient reagents for 8 runs of 3 samples (plus controls) for a maximum of 24 samples per kit.

Full process control

This test requires a full-process negative control. For each run, process a negative control concurrently with the sample(s) beginning with the DNA isolation procedure.

DNA isolation

DNA is isolated from FFPET specimens using the cobas® DNA Sample Preparation Kit (M/N 05985536190).

Macro-dissection

If the sample contains less than 10% tumor content by area, the sample must be macro-dissected as part of the sample preparation.

DNA quantitation

Note: Measurement of DNA concentration should be performed immediately after the DNA isolation procedure and prior to storage.

Note: Store DNA stock according to instructions in **Sample transport, storage, and stability** section.

1. Mix each DNA stock by vortexing for 5 seconds.
2. Quantify DNA using a spectrophotometer according to the manufacturer's protocol. Use **DNA EB** from the **cobas®** DNA Sample preparation kit as the blank for the instrument. An average of two consistent readings is necessary. The two measurements should be within $\pm 10\%$ of each other when the DNA concentration readings are ≥ 20.0 ng/ μ L. For DNA concentration readings < 20.0 ng/ μ L, the two measurements should be within ± 2 ng/ μ L. If the two measurements are not within $\pm 10\%$ of each other when the DNA concentration readings are ≥ 20.0 ng/ μ L or within ± 2 ng/ μ L when the DNA concentration readings are < 20.0 ng/ μ L, an additional 2 readings must be taken until the requirements are met. The average of these two new measurements should then be calculated.

Note: The DNA stock from the processed negative control (**NEG**) does not need to be measured.

3. The DNA stock concentration from the samples must be ≥ 2 ng/ μ L to perform the **cobas** EGFR Test. Three amplification/detections are run per sample, using 25 μ L of a 2 ng/ μ L dilution of DNA stock (total of 50 ng DNA) for each amplification/detection.

Note: Each DNA stock must have a minimum concentration of 2 ng/ μ L to perform the **cobas** EGFR Test. If the concentration of a DNA Stock is < 2 ng/ μ L, repeat the deparaffinization, DNA isolation, and DNA quantitation procedures for that sample using two 5- μ m FFPE sections. For mounted samples, after deparaffinization, combine the tissue from both sections into one tube, immerse the tissue in **TLB + PK** from the **cobas®** DNA Sample Preparation Kit, and perform DNA isolation and quantitation. For unmounted samples, combine the tissue from both sections into one tube and perform deparaffinization, DNA isolation and quantitation. If the DNA stock is still < 2 ng/ μ L, request another FFPE sample section from the referring clinical site.

Amplification and detection

Note: To avoid contamination of working MMX with DNA samples, amplification and detection should be performed in an area separated from DNA isolation. The amplification and detection work area should be thoroughly cleaned before working MMX preparation. For proper cleaning, all surfaces including racks and pipettors should be thoroughly wiped with 0.5% sodium hypochlorite solution followed by wiping with a 70% ethanol solution. Commercial liquid household bleach typically contains sodium hypochlorite at a concentration of 5.25%. A 1:10 dilution of household bleach will produce a 0.5% sodium hypochlorite solution.

Instrument set-up

Refer to the **cobas®** 4800 System – Operator's Manual or **cobas®** 4800 System – User Assistance for detailed instruction for the **cobas® z 480** set up.

Test order set-up

For detailed instructions on the EGFR workflow steps, refer to the **cobas® 4800 System – Operator’s Manual** or **cobas® 4800 System - User Assistance**.

Generate a plate map with the position of all the samples and controls in the run. In a run with only tissue samples, the Mutant Control is loaded into positions **A01 – A03** on the plate. The Negative Control is loaded into positions **B01 – B03** on the plate. Diluted samples are then added in sets of 3 columns, starting from **C01 – C03** through **H10 – H12**, as shown in Figure 2.

The **cobas** EGFR Test can be run in mixed testing mode (e.g., EGFR Tissue with EGFR Plasma). The control positions can vary depending on the tests chosen and the sample numbers. Refer to the **cobas® 4800 System – Operator’s Manual** or **cobas® 4800 System - User Assistance** for more detail of how to set up a mixed test run.

Figure 2 Plate layout for the cobas EGFR Test

Row / Column	01	02	03	04	05	06	07	08	09	10	11	12
A	MC MMX 1	MC MMX 2	MC MMX 3 v2	S7 MMX 1	S7 MMX 2	S7 MMX 3 v2	S15 MMX 1	S15 MMX 2	S15 MMX 3 v2	S23 MMX 1	S23 MMX 2	S23 MMX 3 v2
B	NEG MMX 1	NEG MMX 2	NEG MMX 3 v2	S8 MMX 1	S8 MMX 2	S8 MMX 3 v2	S16 MMX 1	S16 MMX 2	S16 MMX 3 v2	S24 MMX 1	S24 MMX 2	S24 MMX 3 v2
C	S1 MMX 1	S1 MMX 2	S1 MMX 3 v2	S9 MMX 1	S9 MMX 2	S9 MMX 3 v2	S17 MMX 1	S17 MMX 2	S17 MMX 3 v2	S25 MMX 1	S25 MMX 2	S25 MMX 3 v2
D	S2 MMX 1	S2 MMX 2	S2 MMX 3 v2	S10 MMX 1	S10 MMX 2	S10 MMX 3 v2	S18 MMX 1	S18 MMX 2	S18 MMX 3 v2	S26 MMX 1	S26 MMX 2	S26 MMX 3 v2
E	S3 MMX 1	S3 MMX 2	S3 MMX 3 v2	S11 MMX 1	S11 MMX 2	S11 MMX 3 v2	S19 MMX 1	S19 MMX 2	S19 MMX 3 v2	S27 MMX 1	S27 MMX 2	S27 MMX 3 v2
F	S4 MMX 1	S4 MMX 2	S4 MMX 3 v2	S12 MMX 1	S12 MMX 2	S12 MMX 3 v2	S20 MMX 1	S20 MMX 2	S20 MMX 3 v2	S28 MMX 1	S28 MMX 2	S28 MMX 3 v2
G	S5 MMX 1	S5 MMX 2	S5 MMX 3 v2	S13 MMX 1	S13 MMX 2	S13 MMX 3 v2	S21 MMX 1	S21 MMX 2	S21 MMX 3 v2	S29 MMX 1	S29 MMX 2	S29 MMX 3 v2
H	S6 MMX 1	S6 MMX 2	S6 MMX 3 v2	S14 MMX 1	S14 MMX 2	S14 MMX 3 v2	S22 MMX 1	S22 MMX 2	S22 MMX 3 v2	S30 MMX 1	S30 MMX 2	S30 MMX 3 v2

Where: MC= Mutant Control, NEG = Negative Control; S# = sample ID, and MMX # corresponds to Master Mix Reagent 1, 2, or 3 v2.

Note: Any given sample must be spread across three consecutive columns in one row in order to generate a response.

Note: Working Master Mix 1 must be loaded into column 01, 04, 07, and 10 on the plate. Working Master Mix 2 must be loaded into column 02, 05, 08, and 11 on the plate. Working Master Mix 3 v2 must be loaded into column 03, 06, 09, and 12 on the plate.

Note: Up to 30 samples can be loaded onto a single plate. If more than one reagent kit is required to process all of the samples on the plate, then the kits must all be from the same lot.

Dilution calculation of sample DNA stock

Dilution calculation for DNA stock concentrations from 2 ng/μL to 36 ng/μL

Note: DNA stocks from samples should be diluted immediately prior to amplification and detection.

Note: Three amplification/detections are run for each sample requiring a total volume of 75 μL (25 μL for each of three reactions) of a 2 ng/μL dilution of DNA Stock (total of 150 ng DNA).

- For each sample, calculate the volume (μL) of DNA stock needed:

$$\mu\text{L of DNA stock} = (90 \mu\text{L} \times 2 \text{ ng}/\mu\text{L}) \div \text{DNA Stock concentration [ng}/\mu\text{L}]$$
- For each sample, calculate the volume (μL) of **DNA SD** needed:

$$\mu\text{L of DNA SD} = 90 \mu\text{L} - \mu\text{L of DNA Stock}$$

Example:

DNA stock concentration = 6.5 ng/μL

- $\mu\text{L of DNA Stock} = (90 \mu\text{L} \times 2 \text{ ng}/\mu\text{L}) \div 6.5 \text{ ng}/\mu\text{L} = 27.7 \mu\text{L}$
- $\mu\text{L of DNA SD} = (90 \mu\text{L} - 27.7 \mu\text{L}) = 62.3 \mu\text{L}$

Dilution calculation for DNA stock concentrations > 36 ng/μL

Note: DNA Stocks from samples should be diluted immediately prior to amplification and detection.

Note: Three amplification/detections are run for each sample requiring a total volume of 75 μL (25 μL for each of three reactions) of a 2 ng/μL dilution of DNA stock (total of 150 ng DNA).

- At DNA Stock concentrations > 36 ng/μL, use the following formula to calculate the amount of **DNA SD** required to prepare at least 90 μL of diluted DNA stock. This is to ensure that each sample uses a minimum of 5 μL of DNA stock.
- For each sample, calculate the volume (μL) of **DNA SD** needed to dilute 5 μL of DNA stock to 2 ng/μL:

$$\text{Vol. of DNA SD required in } \mu\text{L} = [(5 \mu\text{L of DNA stock} \times \text{DNA stock concentration in ng}/\mu\text{L}) \div 2 \text{ ng}/\mu\text{L}] - 5 \mu\text{L}$$

Example:

DNA stock concentration = 100 ng/μL

- $\text{Vol. of DNA SD required in } \mu\text{L} = [(5 \mu\text{L} \times 100 \text{ ng}/\mu\text{L}) \div 2 \text{ ng}/\mu\text{L}] - 5 \mu\text{L} = 245 \mu\text{L}$
- Use the calculated volume of **DNA SD** to dilute 5 μL of DNA stock.

Sample dilution

- Prepare the appropriate number of 1.5 mL locking-lid microcentrifuge tubes for DNA Dilutions by labeling them with the proper sample identification.
- Using a pipettor with an aerosol-resistant tip, pipette the calculated volumes of **DNA SD** into the respectively labeled tubes. Pipette 45 μL of **DNA SD** into a locking-lid microcentrifuge tube labeled as **NEG**.
- Vortex each DNA stock and the negative control for 5 to 10 seconds.
- Using a pipettor with an aerosol-resistant pipette tip (new tip for each pipetting), gently pipette the calculated volume of each DNA stock into the respective tube containing **DNA SD**. Pipette 45 μL of negative control (extracted eluate) into the **NEG** tube.
- Cap the tubes and vortex each for 5 to 10 seconds.
- Change gloves.

Reaction set-up

Preparation of working master mixes (MMX-1, MMX-2 and MMX-3 v2)

Note: *EGFR MMX-1, EGFR MMX-2, EGFR MMX-3 v2, and working MMX are light-sensitive and must be protected from prolonged exposure to light.*

Note: *Due to the viscosity of the EGFR MMX reagents and working MMX, pipette slowly to ensure all mix is completely dispensed from the tip.*

Note: *The EGFR MMX-1, EGFR MMX-2, and EGFR MMX-3 v2 may appear light blue/purplish. This does not affect the performance of the reagent.*

Prepare three bulk working MMXs, one containing **EGFR MMX-1**, one containing **EGFR MMX-2**, and the other containing **EGFR MMX-3 v2** in separate 1.5 mL locking-lid microcentrifuge tubes.

1. Calculate the volume of **EGFR MMX-1** or **EGFR MMX-2** or **EGFR MMX-3 v2** required for each working MMX using the following formula:

$$\text{Volume of EGFR MMX-1 or EGFR MMX-2 or EGFR MMX-3 v2 required} = (\text{Number of Samples} + 2 \text{ Controls} + 1) \times 20 \mu\text{L}$$

2. Calculate the volume of **MGAC** required for each working MMX using the following formula:

$$\text{Volume of MGAC required} = (\text{Number of Samples} + 2 \text{ Controls} + 1) \times 5 \mu\text{L}$$

Use Table 4 to determine the volume of each reagent needed for the preparation of working MMX based on the number of samples included in the run.

Table 4 Volumes of reagents needed for working MMX-1, working MMX-2 and working MMX-3 v2

		# of Samples*									
		1	2	3	4	5	6	7	8	9	10
MMX	20 μL	80	100	120	140	160	180	200	220	240	260
MGAC	5 μL	20	25	30	35	40	45	50	55	60	65
Total Vol. for Each Working MMX (μL)		100	125	150	175	200	225	250	275	300	325

* Volumes for # of Samples is based on the sum of the # Samples + 2 Controls + 1

3. Remove the appropriate number of **EGFR MMX-1**, **EGFR MMX-2**, **EGFR MMX-3 v2**, and **MGAC** vials from 2°C to 8°C storage. Vortex each reagent for 5 seconds and collect liquid at the bottom of the tube before use. Label a sterile microcentrifuge tube for working MMX-1, working MMX-2, and working MMX-3 v2.
4. Add the calculated volume of **EGFR MMX-1** or **EGFR MMX-2** or **EGFR MMX-3 v2** to their respective working MMX tube.
5. Add the calculated volume of **MGAC** to the working MMX tubes.
6. Vortex the tubes for 3 to 5 seconds to ensure adequate mixing.

Note: *Samples and controls should be added to the AD-plate within 1 hour after the preparation of the working MMXs.*

Note: *Use only cobas® 4800 System AD-plate and Sealing film.*

Preparation of plate

1. Pipette 25 µL of working MMX into each reaction well of the AD-plate that is needed for the run. Do not allow the pipettor tip to touch the plate outside the well.
 - Add working MMX-1 (containing **EGFR MMX-1**) to the AD-plate wells in columns 01, 04, 07, and 10, as needed.
 - Add working MMX-2 (containing **EGFR MMX-2**) to the AD-plate wells in columns 02, 05, 08, and 11, as needed.
 - Add working MMX-3 v2 (containing **EGFR MMX-3 v2**) to the AD-plate wells in columns 03, 06, 09, and 12, as needed.
2. Pipette 25 µL of **EGFR MC** into wells **A01**, **A02**, and **A03** of the AD-plate; mix well using pipette to aspirate and dispense within the well a minimum of two times.
3. Using a new pipettor tip, pipette 25 µL of **NEG** into wells **B01**, **B02**, and **B03** of the AD-plate; mix well using pipette to aspirate and dispense within the well a minimum of two times.

Note: Each run must contain **EGFR MC** in wells **A01**, **A02** and **A03**, and **NEG** in wells **B01**, **B02**, and **B03** or the run will be invalidated by the **cobas® z 480** analyzer.

Note: Change gloves as needed to protect against sample-to-sample contamination and external PCR reaction tube contamination.

4. Using new pipettor tips for each diluted sample DNA, add 25 µL of the first sample DNA to wells **C01**, **C02**, and **C03** of the AD-plate, using a new tip for the addition of the sample DNA to each well; mix each well using a pipette to aspirate and dispense within the well a minimum of two times. Repeat this procedure for the DNA from each sample and follow the template in Figure 2 until all DNA sample dilutions are loaded onto the AD-plate. Ensure that all liquid is collected at the bottom of the wells.
5. Cover the AD-plate with sealing film (supplied with the plates). Use the sealing film applicator to seal the film firmly to the AD-plate.
6. Confirm that all liquid is collected at the bottom of each well before starting PCR.

Note: Amplification and detection should be started within 1 hour after the addition of the first sample DNA dilution to the working MMX.

Starting PCR

Refer to the **cobas® 4800 System – Operator’s Manual** or **cobas® 4800 System - User Assistance** for detailed instructions on the EGFR workflow steps. When the “Select test” pop-up window appears, select “EGFR Tissue P1” and click the “OK” button.

Results

Interpretation of results

Note: All run and sample validation is performed by the cobas® 4800 software.

Note: A valid test run may include both valid and invalid sample results.

For a valid run, sample results are interpreted as shown in Table 5.

Table 5 Result interpretation for the cobas EGFR Test

Test Result	Mutation Result	Interpretation
Mutation Detected	Ex19Del S768I L858R T790M L861Q G719X Ex20Ins (More than one mutation may be present)	Mutation detected in specified targeted EGFR region.
No Mutation Detected (NMD)*	N/A	Mutation not detected in targeted EGFR regions
Invalid	N/A	Sample result is invalid. Repeat the testing of samples with invalid results following the instructions outlined in the “Retesting of samples with invalid results” section below.
Failed	N/A	Failed run due to hardware or software failure. Contact your local Roche office for technical assistance.

* A “No Mutation Detected” result does not preclude the presence of a mutation in the targeted EGFR regions because results depend on percent mutant sequences, adequate sample integrity, absence of inhibitors, and sufficient DNA to be detected.

Result flags may be found under the Result tab (screen) or Flags column (report). Refer to the **Result flags** section for more detail.

Retesting of samples with invalid results

1. Repeat dilution of the invalid sample DNA stock starting from “Dilution Calculation of Sample DNA Stock” and “Sample Dilution” procedures in the **Amplification and detection** section.
2. After performing the DNA stock dilution to 2 ng/μL as described in “Sample Dilution”, continue with “Preparation of working master mix (MMX-1, MMX-2 and MMX-3 v2)” and the remainder of the amplification and detection procedure.

Note: If the sample remains invalid after retesting or there was not enough DNA stock to prepare another dilution in **Retesting of samples with invalid results**, step 1, repeat the entire test procedure for that sample, starting with *Deaffinization and DNA isolation using a new 5-μm FFPE tumor section.*

Quality control and validity of results

One set of **cobas** EGFR Test Mutant Control (**EGFR MC**) (wells **A01**, **A02** and **A03**) and negative control (**NEG**) (wells **B01**, **B02** and **B03**) for working MMX-1, working MMX-2, and working MMX-3 v2 are included in each run of up to 30 samples. A run is valid if the **EGFR MC** and the **NEG** are valid. If an **EGFR MC** or **NEG** is invalid, the entire run is invalid and must be repeated. Prepare a fresh dilution of the previously isolated sample DNA Stock to set up a new AD-plate with controls for amplification and detection.

Mutant control

The **EGFR MC** result must be 'Valid'. If the **EGFR MC** results are consistently invalid, contact your local Roche office for technical assistance.

Negative control

The **NEG** result must be 'Valid'. If the **NEG** results are consistently invalid, contact your local Roche office for technical assistance.

Procedural limitations

1. Test only the indicated specimen types. The **cobas** EGFR Test has been validated for use with NSCLC FFPE tumor samples.
2. The **cobas** EGFR Test has only been validated using the **cobas**® DNA Sample Preparation Kit (Roche P/N: 05985536190).
3. Detection of a mutation is dependent on the number of copies present in the specimen and may be affected by sample integrity, amount of isolated DNA, and the presence of interfering substances.
4. Reliable results are dependent on adequate specimen fixation, transport, storage and processing. Follow the procedures in the **cobas**® DNA Sample Preparation Kit Instructions for Use (M/N 05985536190), in this Instructions for Use, and in the **cobas**® 4800 System – Operator's Manual or **cobas**® 4800 System – User Assistance .
5. The effects of other potential variables such as specimen fixation variables have not been evaluated.
6. The addition of AmpErase enzyme into the **cobas** EGFR Test Master Mix enables selective amplification of target DNA; however, good laboratory practices and careful adherence to the procedures specified in this Instructions For Use are necessary to avoid contamination of reagents.
7. Use of this product must be limited to personnel trained in the techniques of PCR and the use of the **cobas**® 4800 System.
8. Only the **cobas**® z 480 analyzer has been validated for use with this product. No other thermal cycler with real-time optical detection can be used with this product.
9. Due to inherent differences between technologies, it is recommended that, prior to switching from one technology to another, users perform method correlation studies in their laboratory to qualify technology differences.
10. The presence of PCR inhibitors may cause false negative or invalid results.
11. Though rare, mutations within the genomic DNA regions of the EGFR gene covered by the primers or probes used in the **cobas** EGFR Test may result in failure to detect presence of a mutation in exons 18, 19, 20, and 21 (results of "No Mutation Detected").
12. The **cobas** EGFR Test shows cross-reactivity (results of "Mutation Detected") to the exon 19 L747S mutation, a rare acquired mutation that may confer resistance to TKI treatment.¹⁹

13. The **cobas** EGFR Test is validated for use with 50 ng of DNA per reaction well. DNA input amounts lower than 50 ng per reaction well are not recommended.
14. The **cobas** EGFR Test is a qualitative test. The test is not for quantitative measurements of percent mutation.
15. NSCLC FFPET samples containing degraded DNA may affect the ability of the test to detect the EGFR mutations.
16. Samples with results reported as “No Mutation Detected” may harbor EGFR mutations not detected by the assay.
17. The **cobas** EGFR Test detects EGFR mutations in NSCLC patients whose tumors have the exon 18 (G719X) substitutions, exon 19 deletions, exon 20 insertions and substitutions (T790M, S768I) and exon 21 substitutions (L858R, L861Q), but not any other EGFR mutations.

Non-clinical performance evaluation

Note: The study descriptions below include cumulative data performed with v1 and v2 of the **cobas** EGFR Test.

For the non-clinical studies described below, percentage of tumor was assessed by pathology review. Bi-directional Sanger sequencing and next generation sequencing (NGS) were used to select the specimens for testing. Percentage of mutation of NSCLC FFPET specimen was determined using a NGS method.

Analytical sensitivity – limit of blank

To assess performance of the **cobas** EGFR Test in the absence of template and to ensure that a blank sample does not generate an analytical signal that might indicate a low concentration of mutation, samples with no template and NSCLC FFPET EGFR wild-type specimens were evaluated. Using the analysis prescribed in the CLSI EP17-A2 guideline²⁰, the Limit of Blank was determined to be zero for all mutations.

Limit of detection using FFPET specimen blends

Three FFPET specimen DNA extracts for the exon 19 deletion mutations, four FFPET specimen DNA extracts for the L858R mutation, two dual mutant FFPET specimen DNA extracts for L858R and T790M mutations, two FFPET specimen DNA extracts for the G719A mutation, one dual mutant FFPET specimen DNA extract for T790M and G719A, one dual mutant FFPET specimen DNA extract for G719C and S768I mutation, one dual mutant FFPET specimen DNA extract for S768I and G719S, three FFPET specimen DNA extracts for the exon 20 insertion mutation, and three FFPET specimen DNA extracts for the L861Q mutation were blended with EGFR wild-type FFPET specimen extracts to achieve blends with samples targeting 10, 5.0, 2.5 and 1.25% mutation level as determined by a next generation sequencing method (NGS), that was validated for the use for detecting EGFR mutations in exons 18, 19, 20, and 21. Serial dilutions of each specimen blend were prepared and eight replicates of each panel member were run using each of three **cobas** EGFR Test kit lots (n=24/panel member). The limit of detection of each sample was determined by the lowest amount of DNA that gave an EGFR “Mutation Detected” rate of at least 95% for the targeted mutation, shown in Table 6.

Table 6 Limit of detection of the cobas EGFR Test using FFPET specimen blends

EGFR Exon	EGFR Mutation Group	EGFR Nucleic Acid Sequence	Percent Mutation in the Panel Member to achieve ≥ 95% “Mutation Detected” Rate with 50 ng DNA input per reaction well (N = 24 replicates)	COSMIC ID ¹⁴
18	G719X	2156 G>C	2.5	6239
		2156 G>C	4.7	6239
		2155 G>A	3.2	6252
		2155 G>T	5.6	6253
19	Exon 19 Deletion	2235_2249del15	1.4	6223
		2236_2250del15	2.5	6225
		2239_2256del18*	4.7	6255
		2240_2254del15	7.2	12369
		2240_2257del18	13.4**	12370
		2239_2248>C	2.2	12382
		2237_2255>T*	4.1	12384
		2237_2253>TTGCT*	6.3	12416
		2238_2252del15	2.4	23571
		2238_2252del15*	5.5	23571
		2239_2257>GT*	6.0	Not Found
20	T790M	2369 C>T	2.0	6240
		2369 C>T	2.4	6240
		2369 C>T	3.0	6240
	S768I	2303 G>T	1.3	6241
		2303 G>T	2.4	6241
	Exon 20 Insertion	2307_2308insGCCAGCGTG	1.7	12376
		2319_2320insCAC	6.8	12377
2310_2311insGGT		1.3	12378	
21	L858RP	2573 T>G	4.0	6224
		2573 T>G	4.2	6224
		2573 T>G	4.3	6224
		2573 T>G	4.3	6224
		2573 T>G	5.3	6224
	L861Q	2582T>A	2.1	6213
		2582T>A	2.2	6213
		2582T>A	3.4	6213
		2582T>A	3.4	6213

* Only a single level targeting approximately 5% mutation was tested for these non-predominant exon 19 deletion mutations present in the EURTAC cohort. Specimen DNA blends were tested across 3 study sites.

** Limit of Detection of the **cobas** EGFR Test for this mutation is greater than 10% mutation level using the standard input of 50 ng per reaction well.

This study demonstrates that the **cobas** EGFR Test can detect mutations in EGFR exons 18, 19, 20, and 21 with at least 5% mutation level using the standard input of 50 ng per reaction well.

Minimal tumor content

A total of 66 independent EGFR mutant specimens (i.e., 35 of exon 19 deletion mutants and 31 exon 21 L858R mutants) with tumor content ranging from 25% to 99% were tested to determine the minimum tumor content required for detecting the EGFR mutation in NSCLC specimens. None of the specimens evaluated had both an exon 19 deletion mutation and an exon 21 L858R mutation. Each specimen was tested without macrodissection (neat), and after macrodissection. The observed CtR values for the neat and macrodissected slides were analyzed using Deming regression and the Bland-Altman plot (differences vs. mean). The results support the use of specimens whose tumor content is greater than 25% without macrodissection.

An additional 10 EGFR wild-type NSCLC specimens (1-90% tumor content) and 10 EGFR mutant specimens (8-95% tumor content) were tested to determine the whether macro-dissection of low percent tumor NSCLC tumor tissue would improve detectability of the cobas EGFR Test. Each specimen was tested without macro-dissection (neat), and after macro-dissection. All macro-dissected results matched all non-macro-dissected results and the expected mutation and wild-type results were observed for all 20 specimens.

In the Phase III EURTAC trial of erlotinib vs. cisplatin-based chemotherapy, NSCLC FFPET specimens with less than 10% tumor content were macro-dissected prior to EGFR mutation analysis. A subset of the EURTAC screened specimens was evaluated for EGFR mutation status by both the cobas EGFR Test and the next generation sequencing (NGS) methods. Table 7 and Table 8 include NSCLC specimens with valid paired results of EGFR exon 19 or L858R mutations combined from both the cobas EGFR Test and the NGS sequencing. Using the NGS as the reference method, results showed that macro-dissection of NSCLC FFPET sections with less than 10% tumor content demonstrated comparable analytical accuracy to NSCLC FFPET section without macro-dissection.

Together, these studies support that macrodissection is required for NSCLC FFPET sections with less than 10% tumor content prior to testing with the cobas EGFR Test.

Table 7 Performance of the cobas EGFR Test for NSCLC FFPET specimens with tumor contents ≤ 10% (macro-dissected)

Measure of Agreement	Percent Agreement (N)	95% CI
Positive Percent Agreement (PPA)	97.2% (35/36)	85.8%, 99.5%
Negative Percent Agreement (NPA)	94.5% (52/55)	85.1%, 98.1%
Overall Percent Agreement (OPA)	95.6% (87/91)	89.2%, 98.3%

Table 8 Performance of the cobas EGFR Test for NSCLC FFPET specimens with tumor contents > 10% (not macro-dissected)

Measure of Agreement	Percent Agreement (N)	95% CI
Positive Percent Agreement (PPA)	93.0% (107/115)	86.9%, 96.4%
Negative Percent Agreement (NPA)	98.5% (199/202)	95.7%, 99.5%
Overall Percent Agreement (OPA)	96.5% (306/317)	93.9%, 98.1%

Cross-reactivity to other exon 18, 19, 20, and 21 mutations

EURTAC clinical trial specimens

The cobas EGFR Test gave “Mutation Detected” results for the following EGFR mutations observed in the EURTAC clinical trial specimens (Table 9). Analytical performance of the cobas EGFR Test in detecting these mutations has not been evaluated.

Table 9 Mutations observed in the EURTAC cohort determined to cross-react with the cobas EGFR Test

Exon	Mutation Sequence	AA Change	COSMIC ID ¹⁴
19	2236_2252>AT	E746_T751>I	26680
	2239_2253>CAA	L747_T751>Q	51527
	2234_2251>AAT	K745_T751>K	Not Found
	2236_2244del9	E746_R748>E	Not Found
	2236_2263>GAAGCAT	E746_A755>E	Not Found
	2237_2251>AAC	E746_751T>E	Not Found

AURA2 clinical trial specimens

The cobas EGFR Test gave a “Mutation Detected” result for the following EGFR mutation observed in the AURA2 clinical trial specimens (Table 10). Analytical performance of the cobas EGFR Test in detecting this mutation has not been evaluated.

Table 10 Mutations observed in the AURA2 trial determined to cross-react with the cobas EGFR Test

Exon	Mutation Sequence	AA Change	COSMIC ID ¹⁴
21	2572_2573CT>AG	L858R	13553

Specificity – microorganisms and EGFR homologs

Specificity of the cobas EGFR Test was evaluated by testing lung-related microorganisms, and plasmids of EGFR homologs, i.e., plasmids containing the sequences from each of the HER2, HER3, and HER4 genetic regions analogous to the sequences in EGFR exons 18, 19, 20, and 21 amplified by the cobas EGFR Test.

Lung-related microorganisms

Streptococcus pneumoniae and *Haemophilus influenzae* at 4×10^5 colony forming units were found not to cross react or interfere with the cobas EGFR Test when added to specimens containing wild-type and mutant EGFR sequences during the tissue lysis step.

Plasmids of EGFR homologs

Structurally related epidermal receptor tyrosine kinase protein analog sequences (EGFR/HER1, HER2, HER3 and HER4) have been shown not to cross-react with the cobas EGFR Test when the potential cross-reactive sequence was added at a genomic copy number equivalent to 50 ng/PCR input to the isolated DNA stock prior to the amplification/detection procedure. A control condition without plasmid DNA was included. Results indicated that the observed mutations for all 15 tested FFPET specimens matched the expected mutation, as determined by sequencing, in the presence and absence of the added HER gene plasmid DNA. Additionally, the EGFR exon 19 mutation L747S was tested for cross reactivity. Results indicated that the cobas EGFR Test cross-reacts with the EGFR exon 19 mutation L747S.

Interference

Triglycerides (37 mM, CLSI recommended high concentration²¹) and hemoglobin (2 mg/mL, CLSI recommended high concentration²¹) have been shown not to interfere with the **cobas** EGFR Test when the potential interfering substance was added to the lysis step during the specimen preparation procedure.

Albuterol (Ventolin), Ipratropium (Atrovent), Fluticasone (Flonase), Ceftazidime (Fortaz), Imipenem-cilastin (Primaxin), Piperacillin-tazobactam, Cilastin (Cilastatin sodium), Betadine and Lidocaine were shown to not interfere with the performance of the **cobas** EGFR Test when added to the lysis step during the specimen preparation procedure.

Necrotic tissue

NSCLC FFPET specimens with necrotic tissue content up to 60% for EGFR mutant and 85% in wild-type specimens have been shown not to interfere with the call results using the **cobas** EGFR Test.

Repeatability

Repeatability of the **cobas** EGFR Test was assessed using six FFPET specimens, including: two EGFR wild-type specimens; four EGFR mutant specimens, one of each: exon 19 deletion, S768I and G719X, T790M and L858R, and exon 20 insertion mutations. These specimens were tested in duplicate by two operators, using two different reagent lots and two **cobas**® z 480 analyzers over four days. A total of 32 replicates were evaluated per sample. The **cobas** EGFR Test had a correct call rate of 96.9% (186/192).

Repeatability of the **cobas** EGFR Test was also assessed in a second study using four FFPET specimens including: one EGFR wild-type specimens; three EGFR mutant FFPET specimens, one of each: L861Q, G719X, and exon 20 insertion mutations. The specimens were tested in duplicate by two operators, using two different reagent lots and two **cobas**® z 480 analyzers over multiple days. The **cobas** EGFR Test has a correct call accuracy of 99.2% (127/128) across all specimen replicates, operators, reagent lots, and instruments combined.

Specimen handling reproducibility

The reproducibility of the **cobas**® DNA Sample Preparation Kit was examined using sections taken from three FFPET specimen blocks, one containing an exon 19 deletion mutation, one containing an L858R mutation, and one that is wild-type. Each specimen was tested in duplicate at each site on each day. The specimen sections for a given specimen were randomized and tested over a six day period across three sites using one operator at each site, one **cobas**® z 480 analyzer at each site, three **cobas**® DNA Sample Preparation Kit lots, and one **cobas** EGFR Test kit lot. On each test day, each operator isolated and tested the DNA from two NSCLC FFPET curl sections for each specimen using the **cobas** EGFR Test. All specimens reported valid and correct results through-out the six days of testing. For all specimens and operators combined, the **cobas** EGFR Test had a correct call rate of 100% (108/108).

Clinical performance evaluation

Clinical reproducibility study 1

An external study was performed to assess the reproducibility of the **cobas** EGFR Test across 3 external testing sites (2 operators per site), 3 reagent lots, and 5 non-consecutive testing days, with a 13-member panel of DNA samples extracted from FFPET sections of NSCLC wild-type (WT) and Mutant type (MT) tumor specimens. This panel included the L858R mutation in exon 21 and five different exon 19 deletion mutations. Of 92 runs, 90 (97.8%) were valid. A total of 2,340 tests were performed on the 13 panel members in 90 valid runs; all test results were valid. There were no “Mutation Detected” results in 180 valid tests of WT panel members, producing 100% agreement. Agreements were 100% for 10 of the 12 MT panel members. For panel member EX19_2240_2257del18 – 5% Mutation, agreement was 62.8% (67 of 180 test results were No Mutation Detected). For panel member EX19_2240_2257del18 – 10% Mutation, agreement was 99.4% (1 of 180 test result was No Mutation Detected). Results by overall agreement are presented in Table 11. The coefficient of variation (CV) was < 6% in all mutation panel members. Within each panel member, the CV was < 3.5%. For external control the overall CV was < 1.3%. The CV% was < 0.5% for between lots and < 1.2% for within-lot.

Table 11 Overall agreement estimates by panel member in the cobas EGFR Test reproducibility study 1

Panel Member	Number of Valid Tests	Agreement (N)	Agreement % (95% CI) ^a
Wild Type	180	180	100 (98.0, 100.0)
EX19_2235_2249del15 - 5% Mutation	180	180	100 (98.0, 100.0)
EX19_2235_2249del15 - ≤ 10% Mutation	180	180	100 (98.0, 100.0)
EX19_2236_2250del15 - 5% Mutation	180	180	100 (98.0, 100.0)
EX19_2236_2250del15 - ≤ 10% Mutation	180	180	100 (98.0, 100.0)
EX19_2239_2248>C - 5% Mutation	180	180	100 (98.0, 100.0)
EX19_2239_2248>C - ≤ 10% Mutation	180	180	100 (98.0, 100.0)
EX19_2240_2254del15 - 5% Mutation	180	180	100 (98.0, 100.0)
EX19_2240_2254del15 - ≤ 10% Mutation	180	180	100 (98.0, 100.0)
EX19_2240_2257del18 - 5% Mutation	180	113	62.8 (55.3, 69.9)*
EX19_2240_2257del18 - ≤ 10% Mutation	180	179	99.4 (96.9, 100.0)*
EX21_2573T>G=L858R - 5% Mutation	180	180	100 (98.0, 100.0)
EX21_2573T>G=L858R - ≤ 10% Mutation	180	180	100 (98.0, 100.0)

Note: Results were in agreement when a MT panel member had a valid result of “Mutation Detected” or when Wild-type panel member had a valid result of No Mutation Detected.

^a 95% CI = 95% exact binomial confidence interval.

* Analytical sensitivity of the **cobas** EGFR Test for detecting this mutation is greater than 10% mutation level using the standard input of 50 ng per reaction well.

Clinical reproducibility study 2

An external study was performed to assess the reproducibility of the **cobas** EGFR Test across 3 testing sites (2 external and 1 internal, 2 operators per site), 3 reagent lots, and 5 non-consecutive testing days, with an 11-member panel of DNA samples extracted from FFPE sections of NSCLC WT and mutant tumor specimens. This panel included the exon 18 G719X mutation, exon 20 T790M mutation, exon 20 S768I mutation, exon 20 insertion mutation, and exon 21 L861Q mutation. Of 91 runs, 90 (98.9%) were valid. A total of 1,980 tests were performed with 11 panel members tested in duplicate in 90 valid runs; all test results were valid. There were no “Mutation Detected” results in 180 valid tests of WT panel members, producing 100% agreement. Agreements were 100% for all mutant panel members, except for the Exon 20 Insertion LOD panel member. Results by overall agreement are presented in Table 12 below. The CV was < 9.2% in all mutant panel members. For the external control, the overall CV was ≤ 1.3%. The CV was ≤ 0.6% between lots and ≤ 1.1% within-lot.

Table 12 Overall agreement estimates by panel member in the cobas EGFR Test reproducibility study 2

Panel Member	Number of Valid Tests	Agreement (N)	Agreement % (95% CI)*
Wild Type	180	180	100 (98.0, 100.0)
Exon 18 G719X - LOD	180	180	100 (98.0, 100.0)
Exon 20 T790M - LOD	180	180	100 (98.0, 100.0)
Exon 20 S768I - LOD	180	180	100 (98.0, 100.0)
Exon 20 Insertion - LOD	180	166	92.2 (87.3, 95.7)
Exon 21 L861Q - LOD	180	180	100 (98.0, 100.0)
Exon 18 G719X - 2X LOD	180	180	100 (98.0, 100.0)
Exon 20 T790M - 2X LOD	180	180	100 (98.0, 100.0)
Exon 20 S768I - 2X LOD	180	180	100 (98.0, 100.0)
Exon 20 Insertion - 2X LOD	180	180	100 (98.0, 100.0)
Exon 21 L861Q - 2X LOD	180	180	100 (98.0, 100.0)

Note: Results were in agreement when a Mutant Type panel member had a valid result of mutation detected for the target mutation or when a wild-type panel member had a valid result of NMD.

* 95% CI = 95% exact binomial confidence interval.

CI = confidence interval; LOD = limit of detection; NMD = No Mutation Detected

Correlation to reference method using Phase III samples from EURTAC trial

The clinical performance of the **cobas** EGFR Test was assessed by comparing it to two reference methods – 2x bidirectional Sanger sequencing and quantitative next generation sequencing (NGS) – using 487 formalin-fixed paraffin-embedded lung tumor specimens from patients with advanced NSCLC who were screened in the Phase III EURTAC trial of TARCEVA® (erlotinib) vs. cisplatin-based chemotherapy.^{6,22} The clinical and demographic characteristics of the patients whose specimens were available for this retrospective testing were comparable to those of otherwise eligible patients (557) whose specimens were not available for retesting.

A total of 1,276 patients were screened for the EURTAC trial using a combination of laboratory developed tests, collectively referred to as the clinical trial assay (CTA). After excluding ineligible patients and those without CTA results, 1,044 patients were potentially eligible for this study. Among the 1,044 eligible patients, 225 patients had samples that were mutation positive by CTA, 792 had samples that were WT by CTA, and 27 had samples with inconclusive results by CTA. Of the 1,044 potentially eligible patients, 487 specimens were available for retesting with the **cobas** EGFR Test.

All 487 specimens were tested in a blinded fashion with both the **cobas** EGFR Test and Sanger sequencing. Of those, 406 had valid results by both the **cobas** EGFR Test and Sanger sequencing, 38 invalid results were observed by the **cobas** EGFR Test and Sanger sequencing, 38 invalid results by Sanger sequencing only, and 5 invalid results by the **cobas** EGFR Test only. Among the 487 specimens available for retesting with the **cobas** EGFR Test, 444 specimens gave valid **cobas** EGFR Test results and were also tested with NGS. Of those, there were 36 invalid results by NGS; thus, 408 had valid results by both the **cobas** EGFR Test and NGS. The analytical accuracy of the **cobas** EGFR Test compared with each reference method was evaluated by estimating the positive percentage agreement (PPA), negative percentage agreement (NPA), and overall percentage agreement (OPA) and their corresponding 95% CIs for exon 19 deletions and L858R mutations in aggregate, and separately.

In the EURTAC cohort, the **cobas** EGFR Test detected mutations in exon 19 and exon 21 of the EGFR gene as listed in Table 13. Of the mutations detected in the EURTAC cohort, analytical sensitivity was demonstrated on the mutations listed in Table 6.

Table 13 Mutations detected by the cobas EGFR Test in the EURTAC cohort

Exon	Mutation Sequence	AA Change	COSMIC ID ¹⁴
19	2235_2249del15	E746_A750delELREA	6223
	2236_2250del15	E746_A750delELREA	6225
	2239_2256del18	L747_S752delLREATS	6255
	2240_2257del18	L747_P753>S	12370
	2239_2248 TTAAGAGAAG >C	L747_A750>P	12382
	2239_2251>C	L747_T751>P	12383
	2237_2255>T	E746_S752>V	12384
	2237_2253>TTGCT	E746_T751>VA	12416
	2237_2257>TCT	E746_P753>VS	18427
	2238_2252del15	L747_T751delLREAT	23571
	2236_2252>AT	E746_T751>I	26680
	2239_2253>CAA	L747_T751>Q	51527
	2234_2251>AAT	K745_T751>K	Not Found
	2236_2244del9	E746_R748>E	Not Found
	2236_2263>GAAGCAT	E746_A755>E	Not Found
	2237_2251>AAC	E746_T751>E	Not Found
	2239_2257>GT	L747_P753>V	Not Found
21	2573 T>G	L858R	6224

A total of 406 samples with valid **cobas** EGFR Test and Sanger results were included in the agreement analysis. The PPA between the **cobas** EGFR Test and Sanger sequencing was 96.6% (95% CI: 91.5% to 98.7%), and the NPA was 88.3% (95% CI: 84.1% to 91.5%), in the detection of exon 19 deletions and L858R mutations in aggregate as presented in Table 14. The OPA was 90.6%, with the lower limit of the 95% CI above 87%. The PPA, NPA, and OPA in the detection of exon 19 deletion mutations were all > 92%. The PPA, NPA, and OPA in the detection of L858R mutations compared were all > 95%.

Table 14 Comparison of the cobas EGFR Test with Sanger sequencing for the detection of EGFR exon 19 deletion mutations and L858R mutation

Mutation	Measure of Agreement	Percent Agreement (N)	95% CI
Exon 19 Deletion	Positive Percent Agreement (PPA)	97.3% (71/73)	90.5%, 99.2%
	Negative Percent Agreement (NPA)	92.5% (308/333)	89.2%, 94.9%
	Overall Percent Agreement (OPA)	93.3% (379/406)	90.5%, 95.4%
L858R	Positive Percent Agreement (PPA)	95.3% (41/43)	84.5%, 98.7%
	Negative Percent Agreement (NPA)	97.5% (354/363)	95.4%, 98.7%
	Overall Percent Agreement (OPA)	97.3% (395/406)	95.2%, 98.5%
Aggregate	Positive Percent Agreement (PPA)	96.6% (112/116)	91.5%, 98.7%
	Negative Percent Agreement (NPA)	88.3% (256/290)	84.1%, 91.5%
	Overall Percent Agreement (OPA)	90.6% (368/406)	87.4%, 93.1%

A total of 408 samples with valid **cobas** EGFR Test and NGS results were included in the agreement analysis. By comparison, the PPA and NPA between the **cobas** EGFR Test and NGS for the detection of exon 19 deletions and the L858R point mutation in aggregate were 94.0% (95% CI: 89.1% to 96.8%) and 97.7% (95% CI: 95.0% to 98.9%), respectively as presented in Table 15. The OPA was 96.3%, with a lower limit of the 95% CI of 94.0%. The PPA, NPA, and OPA in detecting exon 19 deletion mutations were all > 95%, with all the 95% lower limit CIs > 90%. The PPA, NPA, and OPA in detecting the L858R mutation were also all > 95%, with all lower limits of the 95% CIs ≥ 95% except for PPA (90%), due to the small number of L858R mutations detected.

Table 15 Comparison of the cobas EGFR Test with NGS for the detection of EGFR exon 19 deletion mutations and L858R mutation

Mutation	Measure of Agreement	Percent Agreement (N)	95% CI
Exon 19 Deletion	Positive Percent Agreement (PPA)	95.9% (94/98)	90.0%, 98.4%
	Negative Percent Agreement (NPA)	99.7% (309/310)	98.2%, 99.9%
	Overall Percent Agreement (OPA)	98.8% (403/408)	97.2%, 99.5%
L858R	Positive Percent Agreement (PPA)	90.6% (48/53)	79.7%, 95.9%
	Negative Percent Agreement (NPA)	98.6% (350/355)	96.7%, 99.4%
	Overall Percent Agreement (OPA)	97.5% (398/408)	95.5%, 98.7%
Aggregate	Positive Percent Agreement (PPA)	94.0% (142/151)	89.1%, 96.8%
	Negative Percent Agreement (NPA)	97.7% (251/257)	95.0%, 98.9%
	Overall Percent Agreement (OPA)	96.3% (393/408)	94.0%, 97.8%

Correlation to reference method using Phase II samples from AURA2

The clinical performance of the **cobas** EGFR Test was assessed by comparing it with a validated next generation sequencing (NGS) platform using 383 formalin-fixed paraffin-embedded lung tumor specimens from patients with advanced NSCLC who were screened using the **cobas** EGFR Test in the Phase II AURA2 trial of TAGRISSO® (osimertinib).

A total of 472 patients were screened for the AURA2 trial using the **cobas** EGFR Test. After excluding ineligible patients, 383 patients were eligible for this study.

All 383 specimens were tested in a blinded fashion with both the **cobas** EGFR Test and a validated NGS method. Of those, 368 had valid results by both the **cobas** EGFR Test and NGS. A total of 2 invalid results were observed by both the **cobas** EGFR Test and NGS, 2 invalid results by NGS only, and 11 invalid results by the **cobas** EGFR Test only. The analytical accuracy of the **cobas** EGFR Test compared with the reference method, NGS, for detection of the T790M mutation was evaluated by estimating the positive percent agreement (PPA), negative percent agreement (NPA), and overall percent agreement (OPA), and their corresponding 95% CIs for the T790M mutation.

In the AURA2 trial, the **cobas** EGFR Test detected the mutations of the EGFR gene as listed in Table 16. Of the mutations detected in the AURA 2 trial, analytical sensitivity was demonstrated on the mutations listed in Table 6.

Table 16 Mutations detected by the cobas EGFR Test in the AURA 2 cohort

Exon	Mutation Sequence	AA Change	COSMIC ID ¹⁴
18	2156G>C	G719A	6239
	2155G>A	G719S	6252
	2155G>T	G719C	6253
19	2239_2247delTTAAGAGAA	L747_E749delLRE	6218
	2235_2249del15	E746_A750delELREA	6223
	2236_2250del15	E746_A750delELREA	6225
	2239_2256del18	L747_S752delLREATS	6255
	2240_2254del15	L747_T751delLREAT	12369
	2240_2257del18	L747_P753>S	12370
	2239_2248 TTAAGAGAAG>C	L747_A750>P	12382
	2239_2251>C	L747_T751>P	12383
	2237_2255>T	E746_S752>V	12384
	2237_2251del15	E746_T751>A	12678
	2235_2248>AATTC	E746_A750>IP	13550
	2235_2252>AAT	E746_T751>I	13551
	2253_2276del24	S752_I759delSPKANKEI	13556
2237_2257>TCT	E746_P753>VS	18427	
20	2369C>T	T790M	6240
	2303G>T	S768I	6241
21	2573T>G	L858R	6224
	2573_2574TG>GT	L858R	12429
	2582T>A	L861Q	6213

A total of 368 samples with valid **cobas** EGFR Test and NGS results were included in the agreement analysis. The PPA between the **cobas** EGFR Test and NGS was 88.3% (95% CI: 83.8% to 91.7%), the NPA was 97.3% (95% CI: 92.4% to 99.1%), and the OPA was 91.0% (95% CI: 87.7% to 93.5%) for the detection of the T790M mutation as presented in Table 17. Thirty samples were positive by NGS but negative by the **cobas** EGFR Test: in 10/30 samples, the percent T790M mutation determined by NGS was below LOD (< 2% mutation) of the **cobas** EGFR Test. In 20/30 samples, a moderately delayed IC Ct value indicated poor amplifiability of the DNA template.

Table 17 Comparison of the cobas EGFR Test with NGS for the detection of the EGFR T790M mutation

Measure of Agreement	Percent Agreement (N)	95% CI
Positive Percent Agreement (PPA)	88.3% (226/256)	83.8%, 91.7%
Negative Percent Agreement (NPA)	97.3% (109/112)	92.4%, 99.1%
Overall Percent Agreement (OPA)	91.0% (335/368)	87.7%, 93.5%


Clinical outcome data

EURTAC

The EURTAC trial²² was a Phase III, multicenter, open-label, randomized study of TARCEVA[®] (erlotinib) versus standard platinum doublet chemotherapy as first-line therapy in chemotherapy-naïve patients with advanced NSCLC whose tumors harbored EGFR exon 19 deletions or exon 21 (L858R) substitution mutations, as assessed by a clinical trial assay (CTA). The study was conducted under the sponsorship of the Spanish Lung Cancer Group (SLCG). A total number of 174 patients were enrolled into the study. The trial results showed that patients who received TARCEVA[®] had a statistically significant increase in progression-free survival (PFS) (median PFS 10.4 months vs. 5.1 months) as compared to patients who received chemotherapy, with a hazard ratio of 0.34 ($p < 0.0001$, 95% CI [0.23; 0.49]). The response rate of patients on the TARCEVA[®] arm was greater than the response rate of patients treated with chemotherapy (65.1% vs. 16.1%). No significant difference was observed in overall survival (OS) in the two arms, as 76% of patients on the standard chemotherapy arm crossed over to receive TARCEVA[®].

Of the 174 patients enrolled into the EURTAC trial, 134 cases (77% of the study population, including 69 patients from the TARCEVA[®] arm and 65 patients from the chemotherapy arm) were available for retesting and tested retrospectively by the cobas EGFR Test. Of the 134 cobas EGFR Test retested cases, 116 cases (59 patients from the TARCEVA[®] arm and 57 patients from the chemotherapy arm) were “Mutation Detected” by the cobas EGFR Test. Analysis of the 116 subset revealed that those patients treated with TARCEVA[®] had a significant increase in PFS time (median PFS 10.4 vs. 5.4 months and less likely to have an event of progressive disease or death (HR= 0.34, 95% CI [0.21;0.54], $p < 0.0001$) than patients treated with chemotherapy (Figure 3). The response rate in the TARCEVA[®] arm was greater compared to the chemotherapy arm (59.3% vs. 14.0%). No significant difference in OS was observed between the two groups. The observed clinical benefit in the subset of patients tested with the cobas EGFR Test was comparable to that observed in the full study population (Table 18).

Additional efficacy analysis was conducted to consider patients who were tested positive by the cobas EGFR Test but were tested negative or invalid by the CTA. In the worst case scenario (assuming a hazard ratio of 1 for patients positive by the cobas EGFR Test and negative by CTA), data demonstrated a hazard ratio of 0.42 (95% CI [0.26; 0.57]).

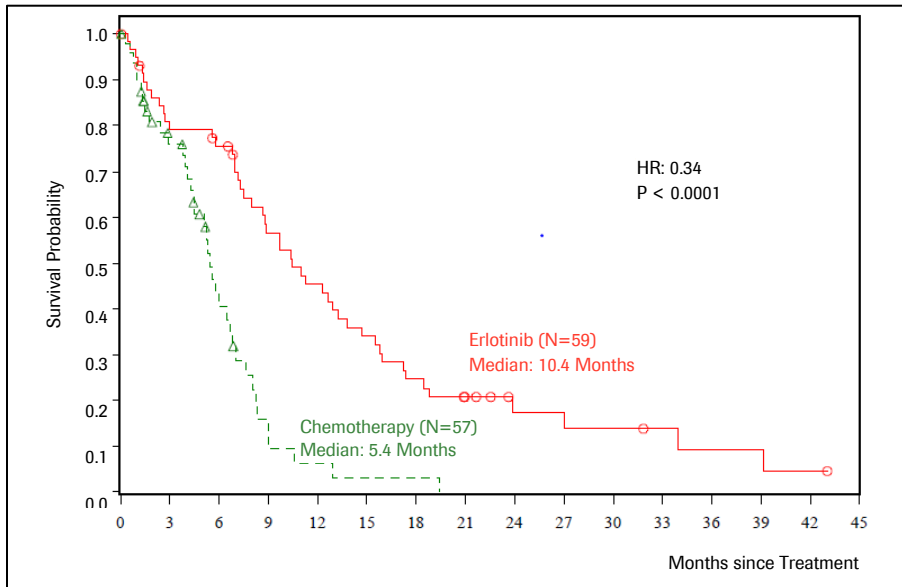Figure 3 Kaplan-Meier plot of PFS by treatment for patients with mutation detected by the cobas EGFR Test (investigator assessment)**Table 18 Clinical benefit of patients tested with the cobas EGFR Test is comparable to that observed in the EURTAC population**

Parameter	cobas EGFR Test PPositive Population n = 116		EURTAC n = 173*	
	Chemotherapy n = 57	Erlotinib n = 59	Chemotherapy n = 87	Erlotinib n = 86
PFS				
Median (Months)	5.4	10.4	5.1	10.4
Hazard Ratio	0.34		0.34	
Hazard Ratio 95% CI	[0.21; 0.54]		[0.23; 0.49]	
P-Value (log-rank test)	< 0.0001		< 0.0001	

* One patient withdrew consent after completion of the EURTAC study, which resulted in a dataset of n = 173.

AURA2

The AURA2 trial²³ was a Phase II, multicenter, open-label, single-arm study, assessing the safety and efficacy of TAGRISSO® (osimertinib) as a second or ≥ third-line therapy in patients with advanced NSCLC, who had progressed following prior therapy with an approved EGFR TKI agent. All patients were required to have T790M mutation-positive NSCLC as detected by the **cobas** EGFR Test. The primary efficacy outcome measure was objective response rate (ORR) according to RECIST 1.1 as evaluated by Blinded Independent Central Review (BICR) using the evaluable for response analysis set. The ORR was defined as the number (%) of patients with at least 1 visit response of complete response (CR) or partial response (PR) that was confirmed at least 4 weeks later (i.e., a best objective response [BOR] of CR or PR).

Of the 472 patients screened for the AURA2 trial, 383 patients were eligible for testing with the **cobas** EGFR Test. Of those eligible, 233 T790M+ patients were recruited into the AURA2 trial, and 210 patients were enrolled and received TAGRISSO® (full analysis set [FAS]).

Table 19 below presents the ORR by BICR and investigator assessment in AURA2. Of 210 patients who received at least one dose of TAGRISSO® (FAS), 128 were confirmed responders by BICR with an ORR of 61.0% (95% CI: 54.0% to 67.6%) and 135 by investigator assessment with an ORR of 64.3% (95% CI: 57.4% to 70.8%).

All 383 patients eligible for AURA2 trial, were retested by the cobas EGFR Test. Of 233 T790M positive patients recruited into the AURA 2 trial, 225 were T790M+ by the cobas EGFR Test and 204 were in the FAS.

Of 204 patients who received TAGRISSO® (FAS), 127 were confirmed responders by BICR with an ORR of 62.3% (95% CI: 55.2% to 68.9%) and 133 by investigator assessment with an ORR of 65.2% (95% CI: 58.2% to 71.7%).

Table 19 Clinical benefit of T790M+ patients tested with the cobas EGFR Test in the AURA2 trial

Analysis Set	Assessed by	AURA2			cobas EGFR Test (IVD) T790M Positive		
		N	Number of Confirmed Responders	ORR (95% CI)	N	Number of Confirmed Responders	ORR (95% CI)
Full Analysis Set (FAS)	Blinded Independent Central Review	210	128	61.0% (54.0%, 67.6%)	204	127	62.3% (55.2%, 68.9%)
	Investigator		135	64.3% (57.4%, 70.8%)		133	65.2% (58.2%, 71.7%)

FLAURA

I. Phase III Trial for TAGRISSO® First-Line

The FLAURA trial¹⁰ was a Phase III, double-blind, randomized clinical trial to assess the efficacy and safety of TAGRISSO® versus standard of care (SoC: EGFR-TKI [either gefitinib or erlotinib]), as first-line treatment in patients with locally advanced or metastatic NSCLC, who had not received previous systemic treatment for advanced disease and whose tumors had locally or centrally confirmed EGFR sensitizing mutations, Ex19del or L858R substitution mutations, collectively referred to as EGFRm positive. The primary endpoint of the FLAURA study was progression-free survival (PFS) based on investigator assessment for patients in the full analysis set (FAS: all globally randomized patients).

A total of 994 patients were screened for randomization in the study, of whom 809 patients had tumor tissue specimens tested by central cobas EGFR Test either prospectively at screening or retrospectively. Of the 556 randomized patients (289 randomized based on the central cobas tissue test and 267 randomized based on a local test), 500 patients were confirmed to have a central cobas EGFRm positive test result. Of the 267 patients randomized based on a local test, 211 patients had a confirmed central cobas EGFRm positive test result, 41 patients did not have a cobas test result due to no/inadequate sample, 9 patients had an invalid cobas test result and 6 patients had a “No Mutation Detected” cobas test result.


Table 20 below presents the HR for PFS by investigator assessment for the full analysis set and the primary device population (patients with a central cobas tissue EGFRm positive result). The HR for PFS by investigator assessment for the full analysis set (N=556), based on a stratified log rank test, was 0.46 (95% CI: 0.37, 0.57). The same point estimate was obtained from an unadjusted Cox proportional hazards model. The HR for PFS by investigator assessment for the primary device population (N=500), calculated from an unadjusted Cox proportional hazards model, was 0.43 (95% CI: 0.34, 0.54). The clinical efficacy observed in the primary device population was consistent with that in the full analysis set. The Kaplan-Meier curve of PFS by investigator assessment in the primary device population is presented in Figure 4.

Table 20 Progression-free survival by investigator assessment for FLAURA full analysis set and for the primary device population (cobas EGFR Test positive)

	FLAURA full analysis set N = 556		FLAURA cobas EGFR Test positive population (Primary Device Population) N = 500	
	Osimertinib (N = 279)	Gefitinib or Erlotinib (N = 277)	Osimertinib (N = 255)	Gefitinib or Erlotinib (N = 245)
PFS				
Number of events (%)	136 (49)	206 (74)	124 (49)	188 (77)
Median PFS in months (95% CI)	18.9 (15.2, 21.4)	10.2 (9.6, 11.1)	18.9 (15.2, 21.4)	9.7 (9.5, 11.0)
Hazard Ratio (95% CI) ^a	0.46 (0.37, 0.57)		0.43 (0.34, 0.54)	
2-sided p-value ^a	<0.0001		<0.001	

^a unadjusted Cox proportional hazards model

Figure 4 Kaplan-Meier Plot of PFS by treatment for patients with mutation detected by the cobas EGFR Test (investigator assessment) in FLAURA

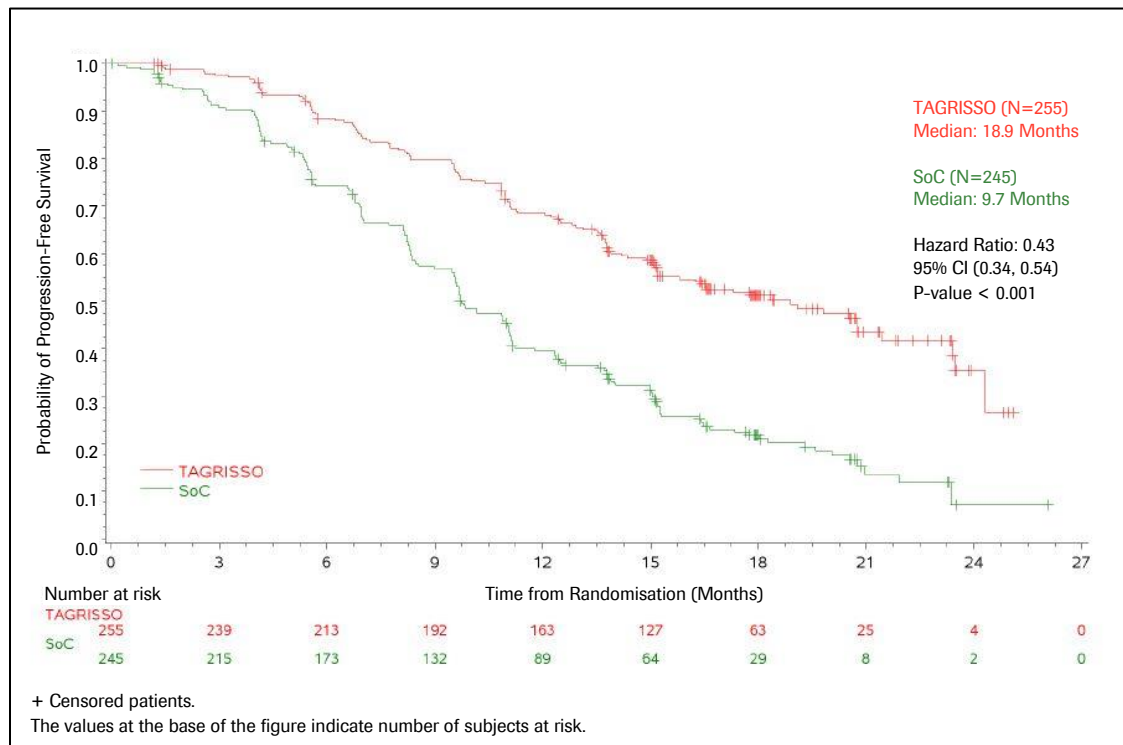

II. IRESSA® Standard of Care Analysis

A separate analysis was performed of tEGFR+ patients treated with IRESSA® (gefitinib) in the control arm of the FLAURA study. Of a total of 178 IRESSA®-treated patients, 174 had an investigator-assessed objective response [ORR=67.8% (118/174, 95% CI: 60.6%, 74.3%, POP0 in Table 21)].

Of the 79 patients treated with IRESSA® and randomized by a central cobas tissue test (the primary efficacy population), 57 had an objective response with an ORR of 72.2% (95% CI: 61.4%, 80.8%, POP1 in Table 21).

The treatment effect of IRESSA®, based on the cobas tissue test, was maintained across other patients patient populations with ORRs ranging from 64.2% (POP2, local test enrolled and also cobas tEGFR+ patients) to 68.5% (POP3, all cobas tEGFR+ patients) (Table 21 and Figure 5). These results are consistent with the results reported for the original registration study (IFUM) for patients selected for IRESSA®.¹³

Table 21 ORR results for different patient populations based on cobas EGFR Test in tissue

Objective Response	Randomized Patients in SoC Arm Treated with IRESSA®				
	Centrally Randomized (cobas tEGFR+)	Locally Randomized (Local tEGFR+)			Total
		cobas tEGFR+	cobas tEGFR-	cobas tEGFR Invalid/Unknown	
No. of Patients	79	70	2	23	174
Response	57	45	1	15	118
Non-Response	22	25	1	8	56
ORR (% , 95% CI)	POP1 = 72.2% (57/ 79: 61.4%, 80.8%)	POP4 = 64.3% (45/ 70: 52.6%, 74.5%)	-	POP5 = 65.2% (15/ 23: 44.9%, 81.2%)	POP0 = 67.8% (118/174: 60.6%, 74.3%)
	-	POP2 = 64.2% (61/ 95: 54.2%, 73.1%)			-
	POP3 = 68.5% (102/149: 60.6%, 75.4%)		-	-	-

Note: Patients with missing objective response were excluded.

Note: tEGFR = tissue EGFR; CI = (score) Confidence Interval.

POP = Population (sub-group)

POP1: ORR for patients randomized by cobas tissue test (primary efficacy population for cobas tissue test).

POP2: ORR for patients randomized by a local tissue test.


POP3: ORR for patients positive by cobas tissue test.

POP4: ORR for patients randomized by a local tissue and confirmed by cobas tissue test.

POP5: ORR for patients randomized by a local tissue test with an invalid or not tested by cobas tissue test.

POP0: ORR for all patients treated with IRESSA®.

Figure 5 Forest plots of ORRs based on cobas EGFR Test in tissue for different populations

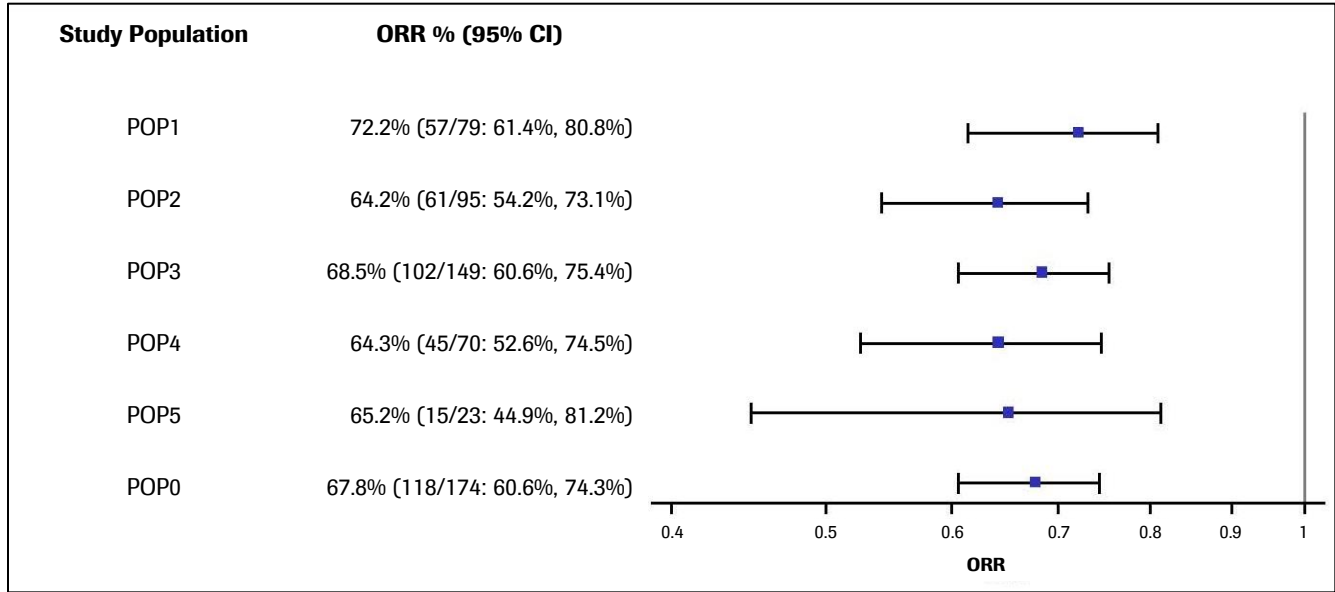

POP = Population (sub-group)

POP1: ORR for patients randomized by **cobas** tissue test (primary efficacy population for **cobas** tissue test).

POP2: ORR for patients randomized by a local tissue test.

POP3: ORR for patients positive by **cobas** tissue test.

POP4: ORR for patients randomized by a local tissue and confirmed by **cobas** tissue test.

POP5: ORR for patients randomized by a local tissue test with an invalid or not tested by **cobas** tissue test.

POP0: ORR for all patients treated with IRESSA®.

SECTION B: FOR USE WITH PLASMA SAMPLES

Sample preparation

Refer to the cobas® cfDNA Sample Preparation Kit (M/N 07247737190) for the isolation of DNA from plasma samples.

Materials and reagents

Materials and reagents provided

Kit/Cassettes	Components and Reagent Ingredients	Quantity per Test	Safety Symbol and Warning
cobas® EGFR Mutation Test v2 Kit 24 Tests (M/N: 07248563190)	EGFR MMX-1 (EGFR Master Mix 1) (M/N: 06471366001) Tris buffer Potassium chloride Glycerol EDTA Tween 20 3.13% Dimethyl sulfoxide 0.09% Sodium azide < 0.10% dNTPs < 0.01% Z05-AS1 DNA polymerase (microbial) < 0.01% AmpErase (uracil-N-glycosylase) enzyme (microbial) < 0.01% Aptamer < 0.01% Upstream and downstream EGFR primers < 0.01% Fluorescent labeled EGFR probes	2 x 0.48 mL	N/A
	EGFR MMX-2 (EGFR Master Mix 2) (M/N: 06471382001) Tris buffer Potassium chloride Glycerol EDTA Tween 20 3.13% Dimethyl sulfoxide 0.09% Sodium azide < 0.10% dNTPs < 0.01% Z05-AS1 DNA polymerase (microbial) < 0.01% AmpErase (uracil-N-glycosylase) enzyme (microbial) < 0.01% Aptamer < 0.01% Upstream and downstream EGFR primers < 0.01% Fluorescent labeled EGFR probes	2 x 0.48 mL	N/A

Kit/Cassettes	Components and Reagent Ingredients	Quantity per Test	Safety Symbol and Warning
cobas® EGFR Mutation Test v2 Kit 24 Tests (M/N: 07248563190)	EGFR MMX-3 v2 (EGFR Master Mix 3) (M/N: 07248601001) Tris buffer Potassium chloride Glycerol EDTA Tween 20 3.13% Dimethyl sulfoxide 0.09% Sodium azide < 0.10% dNTPs < 0.01% Z05-AS1 DNA polymerase (microbial) < 0.01% AmpErase (uracil-N-glycosylase) enzyme (microbial) < 0.01% Aptamer < 0.01% Upstream and downstream EGFR primers < 0.01% Fluorescent labeled EGFR probes	2 x 0.48 mL	N/A
	MGAC (Magnesium acetate) (M/N: 05854326001) Magnesium acetate 0.09% Sodium azide	6 x 0.2 mL	N/A
	EGFR MC (EGFR Mutant Control) (M/N: 06471455001) Tris buffer EDTA Poly-rA RNA (synthetic) 0.05% Sodium azide < 0.1% Plasmid DNA containing EGFR exon 18, 19, 20 and 21 sequences (microbial) < 0.1% EGFR wild-type DNA (cell culture)	6 x 0.1 mL	N/A
	DNA SD (DNA Specimen Diluent) (M/N: 05854474001) Tris-HCl buffer 0.09% Sodium azide	2 x 3.5 mL	N/A

Reagent storage and handling

Reagent	Storage Temperature	Storage Time
cobas® EGFR Mutation Test v2*	2°C to 8°C	Once opened, stable for 4 uses over 90 days or until the expiration date indicated, whichever comes first.

* **EGFR MMX-1, EGFR MMX-2, EGFR MMX-3 v2**, and working MMX (prepared by the addition of **MGAC** to **EGFR MMX-1** or **EGFR MMX-2** or **EGFR MMX-3 v2**) should be protected from prolonged exposure to light. Working MMX must be stored at 2°C to 8°C in the dark. The prepared samples and controls must be added within 1 hour of preparation of the working MMX. Amplification must be started within 1 hour from the time that the processed samples and controls are added to the working MMX.

Additional materials required

Materials	P/N
cobas® cfDNA Sample Preparation Kit	Roche M/N 07247737190
Bleach	Any vendor
70% Ethanol	Any vendor
Sterile disposable, serological 5- and 25-mL pipettes	Any vendor
cobas® 4800 System Microwell Plate (AD-plate) and sealing film	Roche 05232724001
cobas® 4800 System sealing film applicator (supplied with the installation of the cobas® 4800 System)	Roche 04900383001
Adjustable pipettors* (Capable of pipetting 5 – 1000 µL)	Any vendor
Aerosol barrier or positive displacement DNase-free pipette tips	Any vendor
Bench top microcentrifuge* (capable of 20,000 x g)	Eppendorf 5430 or 5430R or equivalent
Freezer capable of -25°C to -15°C storage	Any vendor
Locking-lid microcentrifuge tubes (1.5-mL RNase/DNase free/ PCR grade)	Any vendor
Conical and microcentrifuge tube racks	Any vendor
Vortex mixer*	Any vendor
Disposable powder-free gloves	Any vendor

* All equipment should be maintained according to manufacturer's instructions.

For more information regarding the materials sold separately, contact your local Roche representative.

Instrumentation and software required but not provided

Required Instrumentation and Software, Not Provided
cobas® z 480 analyzer
cobas® 4800 System Control Unit with System Software version 2.2 or higher
EGFR Plasma P1 Analysis Package Software version 1.0 or higher*
Barcode Reader ext USB
Printer

* Refer to the cobas® EGFR Mutation Test v2 kit's Product Information Card (M/N: 07335873001) for the current software version

For more information regarding the materials sold separately, contact your local Roche representative.

Precautions and handling requirements

Warnings and precautions

As with any test procedure, good laboratory practice is essential to the proper performance of this assay.

- For in vitro diagnostic use only
- Safety Data Sheets (SDS) are available upon request from your local Roche office.
- This test is for use with NSCLC plasma samples. Samples should be handled as if infectious using good laboratory procedures such as those outlined in Biosafety in Microbiological and Biomedical Laboratories¹⁶ and in the CLSI Document M29-A4.¹⁷
- The use of sterile disposable pipettes and DNase-free pipette tips is recommended.

Good laboratory practice

- Do not pipette by mouth.
- Do not eat, drink or smoke in laboratory work areas.
- Wash hands thoroughly after handling samples and kit reagents.
- Wear eye protection, laboratory coats and disposable gloves when handling any reagents. Avoid contact of these materials with the skin, eyes or mucous membranes. If contact does occur, immediately wash with large amounts of water. Burns can occur if left untreated. If spills occur, dilute with water before wiping dry.
- Thoroughly clean and disinfect all laboratory work surfaces with a freshly prepared solution of 0.5% sodium hypochlorite in distilled or deionized water (dilute household bleach 1:10). Follow by wiping the surface with 70% ethanol.

Note: Commercial liquid household bleach typically contains sodium hypochlorite at a concentration of 5.25%. A 1:10 dilution of household bleach will produce a 0.5% sodium hypochlorite solution.

Contamination

- Gloves must be worn and must be changed between handling samples and cobas EGFR Test reagents to prevent contamination. Avoid contaminating gloves when handling samples.
- Gloves must be changed frequently to reduce the potential for contamination.
- Gloves must be changed before leaving DNA Isolation areas or if contact with solutions or a sample is suspected.
- Avoid microbial and ribonuclease contamination of reagents.
- The amplification and detection work area should be thoroughly cleaned before working MMX preparation. Supplies and equipment should be dedicated to each activity and not used for other activities or moved between areas. For example, pipettors and supplies used for DNA Isolation must not be used to prepare reagents for amplification and detection.
- It is highly recommended that workflow in the laboratory proceed in a uni-directional manner, completing one activity before proceeding to the next activity. For example, DNA isolation should be completed before starting amplification and detection. DNA isolation should be performed in an area separate from amplification and detection. To avoid contamination of the working master mix with DNA samples, the amplification and detection work area should be thoroughly cleaned before working master mix preparation.

Integrity

- Do not use kits after their expiration dates.
- Do not pool reagents from different kits or lots.
- Do not use disposable items beyond their expiration date.
- All disposable items are for one time use. Do not reuse.
- All equipment should be properly maintained according to the manufacturer's instructions.

Disposal

- DNA EB, MGAC, EGFR MMX-1, EGFR MMX-2, EGFR MMX-3 v2, EGFR MC, and DNA SD contain sodium azide. Sodium azide may react with lead and copper plumbing to form highly explosive metal azides. While disposing of sodium azide containing solutions down laboratory sinks, flush the drains with a large volume of cold water to prevent azide buildup.
- Dispose of unused reagents and waste in accordance with country, federal, state and local regulations.

Spillage and cleaning

- If spills occur on the cobas® 4800 instrument, follow the instructions in the appropriate cobas® 4800 System – Operator’s Manual or cobas® 4800 System – User Assistance to clean.
- Do not use sodium hypochlorite solution (bleach) for cleaning the cobas® z 480 analyzer. Clean the cobas® z 480 analyzer according to procedures described in the appropriate cobas® 4800 System – Operator’s Manual or cobas® 4800 System – User Assistance.
- For additional warnings, precautions and procedures to reduce the risk of contamination for the cobas® z 480 analyzer, consult the cobas® 4800 System – Operator’s Manual or cobas® 4800 System – User Assistance.

Sample collection, transport, and storage

Note: Handle all samples as if they are capable of transmitting infectious agents.

Sample collection and handling

Roche Cell-Free DNA Collection Tube

Plasma from whole blood collected in Roche Cell-Free DNA Collection Tubes (Roche cfDNA tubes) has been validated for use with the cobas EGFR Test.

Plasma should be separated from blood collected in the Roche cfDNA tube within 7 days of collection. Blood samples collected in the Roche cfDNA tube are stable for 7 days when stored or shipped between 15-25°C, with transient excursions of up to 16 hours to 15-30°C. After separation of plasma, store as indicated in **Sample transport, storage and stability** section below.

Note: Hemolysis has been observed in plasma separated from blood collected in the Roche cfDNA tube. However, hemoglobin concentrations at ≤ 2.0 g/L have been shown not to interfere with the performance of the cobas EGFR Test.

K2 EDTA Collection Tube

Plasma from whole blood collected in K2 EDTA tubes has been validated for use with the cobas EGFR Test.

K2 EDTA whole blood may be stored for up to 8 hours at $\leq 30^\circ\text{C}$. After separation of plasma, store as indicated in the **Sample transport, storage and stability** section below.

Sample transport, storage and stability

Transportation of plasma samples must comply with country, federal, state, and local regulations for the transport of etiologic agents.¹⁸

Plasma samples are stable for one of the following:

Plasma Sample Storage Temperature	$\leq -70^\circ\text{C}$	-15°C to -25°C	2°C to 8°C	15°C to 30°C
Storage Time for Roche cfDNA Plasma	Up to 30 days	Up to 30 days	Up to 7 days	Up to 1 day
Storage Time for K2 EDTA Plasma	Up to 12 months	Up to 12 months	Up to 3 days	Up to 1 day

Processed sample storage and stability

Processed sample (extracted cfDNA) from plasma derived from the Roche cfDNA tube or K2 EDTA tube is stable for one of the following:

Extracted cfDNA Storage Temperature	-15°C to -25°C	2°C to 8°C	15°C to 30°C
Storage Time	Up to 2 freeze thaws over 60 days	Up to 21 days	Up to 7 days

Extracted cfDNA should be used within the recommended storage periods or before the expiration date of the cobas® cfDNA Sample Preparation Kit used to extract the DNA, whichever comes first.

Prior to using extracted, stored DNA stocks, pulse vortex and centrifuge the elution tube containing the stock.

Test procedure

Running the test

Figure 6 cobas EGFR Test workflow with cobas® cfDNA Sample Preparation Kit

1	Start the system
2	Perform instrument maintenance
3	Remove samples and reagents from storage
4	Prepare samples for binding to column
5	Perform DNA isolation
6	Elute DNA
7	Create work order and print plate layout
8	Prepare amplification reagents
9	Load AD-plate with amplification reagents
10	Load AD-plate with sample
11	Seal AD-plate
12	Load AD-plate on the cobas® z 480 analyzer
13	Start the run
14	Review results
15	With LIS: send results to LIS
16	Unload analyzer

Instructions for use

Note: Only plasma separated from blood collected in the Roche cfDNA tube or in a K2 EDTA tube is validated for use with the cobas EGFR Test.

Note: Refer to the cobas® z 480 analyzer Instrument Manual for detailed operating instructions for the cobas® z 480 analyzer.

Run size

A single run can include from 1 to 30 samples (plus controls) per 96-well AD-plate. When running more than 24 samples, multiple cobas EGFR Test kits will be required.

The cobas EGFR Test kit contains sufficient reagents for 8 runs of 3 samples (plus controls) for a maximum of 24 samples per kit.

Full process control

This test requires a full process negative control. For each run, process a negative control concurrently with the sample(s) beginning with the DNA isolation procedure.

DNA isolation

DNA is isolated from plasma samples using the cobas® cfDNA Sample Preparation Kit (M/N 07247737190).

Amplification and detection

Note: To avoid contamination of working MMX with DNA samples, amplification and detection should be performed in an area separated from DNA Isolation. The amplification and detection work area should be thoroughly cleaned before working MMX preparation. For proper cleaning, all surfaces including racks and pipettors should be thoroughly wiped with 0.5% sodium hypochlorite solution followed by wiping with a 70% ethanol solution. Commercial liquid household bleach typically contains sodium hypochlorite at a concentration of 5.25%. A 1:10 dilution of household bleach will produce a 0.5% sodium hypochlorite solution.

Instrument set-up

Refer to the cobas® 4800 System – Operator’s Manual or cobas® 4800 System - User Assistance for detailed instruction for the cobas® z 480 set up.

Test order set-up

For detailed instructions on the EGFR workflow steps, refer to the cobas® 4800 System – Operator’s Manual or cobas® 4800 System - User Assistance.

Generate a plate map with the position of all the samples and controls in the run. In a run with only plasma samples, the Mutant Control is loaded into positions **A01 – A03** on the plate. The Negative Control is loaded into positions **B01 – B03** on the plate. Samples are then added in sets of 3 columns, starting from **C01 – C03** through **H10 – H12**, as shown in Figure 7.

The cobas EGFR Test can be run in mixed testing mode (e.g. EGFR Tissue with EGFR Plasma). The control positions can vary depending on the tests chosen and the sample numbers. Refer to Software Operator’s Manual for the cobas® EGFR Mutation Test v2 or cobas® 4800 System – Operator’s Manual or cobas® 4800 System - User Assistance for more detail of how to set up a mixed test run.

Figure 7 Plate layout for the cobas EGFR Test

Row / Column	01	02	03	04	05	06	07	08	09	10	11	12
A	MC MMX 1	MC MMX 2	MC MMX 3 v2	S7 MMX 1	S7 MMX 2	S7 MMX 3 v2	S15 MMX 1	S15 MMX 2	S15 MMX 3 v2	S23 MMX 1	S23 MMX 2	S23 MMX 3 v2
B	NEG MMX 1	NEG MMX 2	NEG MMX 3 v2	S8 MMX 1	S8 MMX 2	S8 MMX 3 v2	S16 MMX 1	S16 MMX 2	S16 MMX 3 v2	S24 MMX 1	S24 MMX 2	S24 MMX 3 v2
C	S1 MMX 1	S1 MMX 2	S1 MMX 3 v2	S9 MMX 1	S9 MMX 2	S9 MMX 3 v2	S17 MMX 1	S17 MMX 2	S17 MMX 3 v2	S25 MMX 1	S25 MMX 2	S25 MMX 3 v2
D	S2 MMX 1	S2 MMX 2	S2 MMX 3 v2	S10 MMX 1	S10 MMX 2	S10 MMX 3 v2	S18 MMX 1	S18 MMX 2	S18 MMX 3 v2	S26 MMX 1	S26 MMX 2	S26 MMX 3 v2
E	S3 MMX 1	S3 MMX 2	S3 MMX 3 v2	S11 MMX 1	S11 MMX 2	S11 MMX 3 v2	S19 MMX 1	S19 MMX 2	S19 MMX 3 v2	S27 MMX 1	S27 MMX 2	S27 MMX 3 v2
F	S4 MMX 1	S4 MMX 2	S4 MMX 3 v2	S12 MMX 1	S12 MMX 2	S12 MMX 3 v2	S20 MMX 1	S20 MMX 2	S20 MMX 3 v2	S28 MMX 1	S28 MMX 2	S28 MMX 3 v2
G	S5 MMX 1	S5 MMX 2	S5 MMX 3 v2	S13 MMX 1	S13 MMX 2	S13 MMX 3 v2	S21 MMX 1	S21 MMX 2	S21 MMX 3 v2	S29 MMX 1	S29 MMX 2	S29 MMX 3 v2
H	S6 MMX 1	S6 MMX 2	S6 MMX 3 v2	S14 MMX 1	S14 MMX 2	S14 MMX 3 v2	S22 MMX 1	S22 MMX 2	S22 MMX 3 v2	S30 MMX 1	S30 MMX 2	S30 MMX 3 v2

Where: MC= Mutant Control, NEG = Negative Control S# = sample ID, and MMX # corresponds to Master Mix Reagent 1, 2, or 3 v2.

Note: Any given sample must be spread across three consecutive columns in one row in order to generate a response.

Note: Working Master Mix 1 must be loaded into column 01, 04, 07, and 10 on the plate. Working Master Mix 2 must be loaded into column 02, 05, 08, and 11 on the plate. Working Master Mix 3 v2 must be loaded into column 03, 06, 09, and 12 on the plate.

Note: Up to 30 samples can be loaded onto a single plate. If more than one reagent kit is required to process all of the samples on the plate, then the kits must all be from the same lot.

Reaction set-up

Preparation of working master mix (MMX-1, MMX-2 and MMX-3 v2)

Note: EGFR MMX-1, EGFR MMX-2, EGFR MMX-3 v2, and working MMX are light-sensitive and must be protected from prolonged exposure to light.

Note: Due to the viscosity of the EGFR MMX reagents and working MMX, pipette slowly to ensure all mix is completely dispensed from the tip.

Note: The EGFR MMX-1, EGFR MMX-2, and EGFR MMX-3 v2 may appear light blue/purplish. This does not affect the performance of the reagent.

Note: Prepare three bulk working MMXs, one containing EGFR MMX-1, one containing EGFR MMX-2, and the other containing EGFR MMX-3 v2 in separate 1.5 mL microcentrifuge tubes.

1. Calculate the volume of EGFR MMX-1 or EGFR MMX-2 or EGFR MMX-3 v2 required for each working MMX using the following formula:

$$\text{Volume of EGFR MMX-1 or EGFR MMX-2 or EGFR MMX-3 v2 required} = (\text{Number of Samples} + 2 \text{ Controls} + 1) \times 20 \mu\text{L}$$

2. Calculate the volume of MGAC required for each working MMX using the following formula:

$$\text{Volume of MGAC required} = (\text{Number of Samples} + 2 \text{ Controls} + 1) \times 5 \mu\text{L}$$

Use Table 22 to determine the volume of each reagent needed for the preparation of working MMX based on the number of samples included in the run.

Table 22 Volumes of reagents needed for working MMX-1, working MMX-2 and working MMX-3 v2

		# of Samples*									
		1	2	3	4	5	6	7	8	9	10
MMX	20 μL	80	100	120	140	160	180	200	220	240	260
MGAC	5 μL	20	25	30	35	40	45	50	55	60	65
Total Vol. for Each Working MMX (μL)		100	125	150	175	200	225	250	275	300	325

* Volumes for # of Samples is based on the sum of the # Samples + 2 Controls + 1

3. Remove the appropriate number of EGFR MMX-1, EGFR MMX-2, EGFR MMX-3 v2, and MGAC vials from 2°C to 8°C storage. Vortex each reagent for 5 seconds and collect liquid at the bottom of the tube before use. Label a sterile microcentrifuge tube for working MMX-1, working MMX-2, and working MMX-3 v2.
4. Add the calculated volume of EGFR MMX-1 or EGFR MMX-2 or EGFR MMX-3 v2 to their respective working MMX tube.
5. Add the calculated volume of MGAC to the working MMX tubes.
6. Vortex the tubes for 3 to 5 seconds to ensure adequate mixing.

Note: Samples and controls should be added to the AD-plate within 1 hour after the preparation of the working MMXs.

Note: Use only cobas® 4800 System AD-plate and Sealing film.

Preparation of plate

Note: If using stored DNA stocks, follow the instructions in **Sample transport, storage and stability** section.

1. Pipette 25 µL of working MMX into each reaction well of the AD-plate that is needed for the run. Do not allow the pipettor tip to touch the plate outside the well.
 - Add working MMX-1 (containing **EGFR MMX-1**) to the AD-plate wells in columns 01, 04, 07, and 10, as needed.
 - Add working MMX-2 (containing **EGFR MMX-2**) to the AD-plate wells in columns 02, 05, 08, and 11, as needed.
 - Add working MMX-3 v2 (containing **EGFR MMX-3 v2**) to the AD-plate wells in columns 03, 06, 09, and 12, as needed.
2. Pipette 25 µL of **EGFR MC** into wells **A01**, **A02**, and **A03** of the AD-plate; mix well using pipette to aspirate and dispense within the well a minimum of two times.
3. Using a new pipettor tip, pipette 25 µL of **NEG** into wells **B01**, **B02**, and **B03** of the AD-plate; mix well using pipette to aspirate and dispense within the well a minimum of two times.

Note: Each run must contain **EGFR MC** in wells **A01**, **A02** and **A03**, and **NEG** in wells **B01**, **B02**, and **B03** or the run will be invalidated by the **cobas® z 480** analyzer.

Note: Change gloves as needed to protect against sample-to-sample contamination and external PCR reaction tube contamination.

4. Using new pipettor tips for each sample DNA, add 25 µL of the first sample DNA to wells **C01**, **C02**, and **C03** of the AD-plate, using a new tip for the addition of the sample DNA to each well; mix each well using a pipette to aspirate and dispense within the well a minimum of two times. Repeat this procedure for the DNA from each sample and follow the template in Figure 7 until all DNA samples are loaded onto the AD-plate. Ensure that all liquid is collected at the bottom of the wells.

Note: Prior to using stored DNA stocks, pulse vortex and centrifuge the elution tube containing the stock.

5. Cover the AD-plate with sealing film (supplied with the plates). Use the sealing film applicator to seal the film firmly to the AD-plate.
6. Confirm that all liquid is collected at the bottom of each well before starting PCR.

Note: Amplification and detection should be started within 1 hour after the addition of the first sample DNA dilution to the working MMX.

Starting PCR

Refer to the **cobas® 4800 System – Operator’s Manual** or **cobas® 4800 System - User Assistance** for detailed instructions on the EGFR workflow steps. When the “Select test” pop-up window appears, select “EGFR Plasma P1” and click the “OK” button.

Results

Interpretation of results

Note: All run and sample validation is performed by the cobas® 4800 software.

Note: A valid test run may include both valid and invalid sample results.

For a valid run, sample results are interpreted as shown in Table 23.

Table 23 Result interpretation for the cobas EGFR Test

Test Result	Mutation Result	Semi-Quantitative Index (SQI) Result	Interpretation
Mutation Detected	Ex19Del S768I L858R T790M L861Q G719X Ex20Ins (More than one mutation may be present)	Ex19Del: SQI S768I: SQI L858R: SQI T790M: SQI L861Q: SQI G719X: SQI Ex20Ins: SQI (More than one mutation may be present)	Mutation detected in specified targeted EGFR region.
No Mutation Detected (NMD)*	N/A	N/A	Mutation not detected in targeted EGFR regions
Invalid	N/A	N/A	Sample result is invalid. Repeat the testing of samples with invalid results following the instructions outlined in the “ Retesting of samples with invalid results ” section below.
Failed	N/A	N/A	Failed run due to hardware or software failure. Contact your local Roche office for technical assistance

* A “No Mutation Detected” result does not preclude the presence of a mutation in the targeted EGFR regions because results depend on concentration of mutant sequences, adequate sample integrity, absence of inhibitors, and sufficient DNA to be detected.

Result flags may be found under the Result tab (screen) or Flags column (report). Refer to **Result flags** section for more detail.

Semi Quantitative Index (SQI)

The SQI is a semi-quantitative measure of the amount of mutant cfDNA in a sample that can be used to measure differences in mutation load over time. An increase in the SQI value indicates an increase in the amount of the corresponding target mutation within an individual sample source, whereas a decrease in the SQI value indicates a decrease in the overall amount of the corresponding target mutation within an individual sample source. Representative SQI results for each EGFR mutation class detected by the test are shown in the linearity results in Figure 8 – Figure 14.

Retesting of samples with invalid results

1. If the run is invalid, there will be insufficient volume of extracted DNA for each sample to repeat Amplification and Detection. Repeat the entire test procedure for all samples, starting with DNA isolation.
2. If the run is valid but the sample is invalid, there will be insufficient volume of extracted DNA for each sample to repeat Amplification and Detection. Repeat the entire test procedure for the invalid sample, starting with DNA isolation.

Quality control and validity of results

One set of **cobas** EGFR Test Mutant Control (**EGFR MC**) (wells **A01**, **A02** and **A03**) and negative control (**NEG**) (wells **B01**, **B02** and **B03**) for working MMX-1, working MMX-2, and working MMX-3 v2 are included in each run of up to 30 samples. A run is valid if the **EGFR MC** and the **NEG** are valid. If an **EGFR MC** or **NEG** is invalid, the entire run is invalid and must be repeated.

Mutant control

The **EGFR MC** result must be 'Valid'. If the **EGFR MC** results are consistently invalid, contact your local Roche office for technical assistance.

Negative control

The **NEG** result must be 'Valid'. If the **NEG** results are consistently invalid, contact your local Roche office for technical assistance.

Procedural limitations

1. Test only the indicated sample types. The **cobas** EGFR Test has been validated for use with plasma separated from blood collected in the Roche cfDNA tube or K2 EDTA tube.
2. The **cobas** EGFR Test performance was validated using the **cobas**® cfDNA Sample Preparation Kit.
3. Detection of a mutation is dependent on the number of copies present in the sample and may be affected by sample integrity, amount of isolated DNA, and the presence of interfering substances.
4. Reliable results are dependent on adequate transport, storage and processing. Follow the procedures in these Instructions for Use and in the **cobas**® 4800 System – Operator's Manual or **cobas**® 4800 System - User Assistance.
5. Pipetting from the bottom of the elution tube may disrupt the pellet and adversely affect test results.
6. The addition of AmpErase enzyme into the **cobas** EGFR Test Master Mix enables selective amplification of target DNA; however, good laboratory practices and careful adherence to the procedures specified in these Instructions for Use are necessary to avoid contamination of reagents.
7. Use of this product must be limited to personnel trained in the techniques of PCR and the use of the **cobas**® 4800 System.
8. Only the **cobas**® z 480 analyzer has been validated for use with this product. No other thermal cycler with real-time optical detection can be used with this product.
9. Due to inherent differences between technologies, it is recommended that, prior to switching from one technology to another, users perform method correlation studies in their laboratory to qualify technology differences.
10. The presence of PCR inhibitors may cause false negative or invalid results.
11. Though rare, mutations within the genomic DNA regions of the EGFR gene covered by the primers or probes used in the **cobas** EGFR Test may result in failure to detect the presence of a mutation in exons 18, 19, 20, and 21 (results of "No Mutation Detected").

12. The **cobas** EGFR Test shows cross-reactivity (results of “Mutation Detected”) to the exon 19 L747S mutation, a rare acquired mutation that may confer resistance to TKI treatment.¹⁹
13. Samples tested at high concentrations ($>10^5$ copies/mL) may generate false results.
14. The **cobas** EGFR Test was validated for use with 25 μ L of DNA stock per reaction well. DNA stock input volumes lower than 25 μ L per reaction well are not recommended.
15. The procedure described above must be followed to detect ≥ 100 copies of mutant DNA per mL of plasma separated from blood collected in the Roche cfDNA tube or in K2 EDTA tube for the EGFR mutations in Table 3.
16. Samples with results reported as “No Mutation Detected” may harbor EGFR mutations not detected by the assay.
17. Consideration should be made for a “No Mutation Detected” result in plasma to reflex to or be confirmed by tissue testing.
18. The plasma derived from whole blood collected in the Roche cfDNA tube is sufficient for one time testing only.
19. Plasma from patient draws not drawn at the same time should not be combined.
20. Performance of the **cobas** EGFR Test has not been established with clotted samples collected with the Roche cfDNA tube. Clotted samples should be rejected and a new sample drawn from the patient.
21. Hemolysis has been observed in plasma separated from blood collected in the Roche cfDNA tube. Hemoglobin concentrations at > 2.0 g/L may interfere with the performance of the **cobas** EGFR Test.

Non-clinical performance evaluation

Analytical performance

The following data is intended to demonstrate the analytical performance of the **cobas** EGFR Test.

Analytical sensitivity – limit of blank

To assess performance of the **cobas** EGFR Test in the absence of template and to ensure that a blank sample does not generate an analytical signal that might indicate a low concentration of mutation, samples of healthy-donor K2 EDTA plasma EGFR wild-type samples were evaluated. Using the analysis prescribed in the CLSI EP17-A2 guideline²⁰, the Limit of Blank was determined to be zero for all mutations.

Limit of detection using cell line DNA

K2 EDTA plasma

Cell line DNAs containing each of the seven mutation classes detected by the test were added to healthy-donor K2 EDTA plasma that was wild-type for EGFR. Serial dilutions were prepared and 24 replicates of each panel member were tested, using each of three **cobas** EGFR Test kit lots.

Limit of Detection was determined for each the seven mutation classes detected by the test as the lowest concentration of DNA that gave an EGFR “Mutation Detected” rate of at least 95% for the targeted mutation. The results are shown in Table 24.

Table 24 Limit of detection of **cobas** EGFR Test with K2 EDTA Plasma

EGFR Exon	EGFR Mutation Group	EGFR Nucleic Acid Sequence	Intact* DNA LOD (copies/mL)	Sheared** DNA LOD (copies/mL)	COSMIC ID ¹⁴
18	G719A	2156G>C	100	100	6239
19	Ex19Del	2235_2249del15	25	75	6223
20	T790M	2369C>T	25	100	6240
20	S768I	2303G>T	20	25	6241
20	Ex20Ins	2307_2308ins9GCCAGCGTG	80	25	12376
21	L858R	2573T>G	10	100	6224
21	L861Q	2582T>A	30	30	6213

The differences in observed LOD are due to the difference in background DNA.

* Intact cell line DNA had a WT DNA background of approximately 10,000 copies/mL.

** Cell line DNA, mechanically sheared to an average size of 220bp, had a WT DNA background of approximately 100,000 copies/mL.

Roche cfDNA plasma

For plasma separated from blood collected in the Roche cfDNA tube, the LOD values were verified by adding sheared cell line DNAs containing each of the seven mutation classes detected by the test to healthy-donor Roche cfDNA plasma that was wild-type for EGFR. Dilutions were prepared targeting the LOD concentrations indicated in Table 24 and 20 replicates for each sample were tested using one **cobas** EGFR Test kit lot. The observed hit rate for each mutation was 100%.

In summary, the **cobas** EGFR Test can detect mutations in EGFR exons 18, 19, 20, and 21 with ≤ 100 copies of mutant DNA per mL of plasma using the standard input of 25 μ L of DNA stock per reaction well with either K2 EDTA or Roche cfDNA plasma.

Cross reactivity to other Exon 18, 19, 20, and 21 mutations

AURA Extension and AURA2 clinical trial samples

The cobas EGFR Test gave “Mutation Detected” results for the following EGFR mutations observed in the AURA Extension and AURA2 clinical trial samples (Table 25). The AURA Extension study was used to supplement the samples in the AURA2 cohort and increase the likelihood of detecting rare mutations in plasma. Analytical performance of the cobas EGFR Test in detecting these mutations has not been evaluated.

Table 25 Mutations observed in the AURA Extension and AURA2 Trial determined to cross-react with the cobas EGFR Test

Exon	Mutation Sequence	AA Change	COSMIC ID ¹⁴
19	2236_2256>ATC	E746_S752>I	133190
	2237_2258>TATC	E746_P753>VS	Not Found
	2239_2256>CAG	L747_S752>Q	Not Found
	2239_2264>GCCAA	L747_A755>AN	85891
	2240_2264>CGAGAGA	L747_A755>SRD	Not Found

Specificity – microorganism

Specificity of the cobas EGFR Test was evaluated by testing *Staphylococcus epidermidis* at 1×10^6 colony forming units, which was found not to cross react or interfere with the cobas EGFR Test when added to healthy-donor K2 EDTA plasma samples containing wild-type and mutant EGFR sequences.

Interference

K2 EDTA plasma

Triglycerides (37 mM CLSI, recommended high concentration²¹), 0.2 g/L of bilirubin (unconjugated or conjugated, CLSI recommended high concentration²¹), and hemoglobin (1.5 g/L) have been shown not to interfere with the cobas EGFR Test when the potentially interfering substance was added to healthy-donor K2 EDTA plasma samples containing wild-type and mutant EGFR sequences. Hemoglobin at a concentration of 2.0 g/L in plasma has been shown to interfere with the cobas EGFR Test. Albumin at a concentration of ≥ 60 g/L (60 g/L, CLSI recommended high concentration²¹) may interfere with the cobas EGFR Test.

The study results demonstrate that EDTA, Neupogen, and TARCEVA® do not interfere with the performance of the cobas EGFR Test when the potentially interfering substance was added to healthy-donor K2 EDTA plasma samples containing wild-type and mutant EGFR sequences.

Roche cfDNA plasma

Triglycerides (37 mM, CLSI recommended high concentration²¹), 0.2 g/L of bilirubin (unconjugated or conjugated, CLSI recommended high concentration²¹), hemoglobin (2.0 g/L), and albumin (60 g/L, CLSI recommended high concentration²¹) have been shown not to interfere with the cobas EGFR Test when the potentially interfering substance was added to samples containing wild-type and mutant EGFR sequences in healthy-donor Roche cfDNA plasma.

Linearity

K2 EDTA plasma


The linearity study of cobas EGFR Test was performed with dilution series of at least 8 panel members spanning the linear range for the predominant mutation for each EGFR mutation class reported by the test. Panel members were prepared by diluting cell line DNAs containing each of predominant mutations into healthy-donor K2 EDTA plasma that is wild-type for EGFR. The evaluation was performed according to CLSI Guideline EP-06A.²⁴ Ten replicates per panel member for each of 2 lots were tested for concentrations up to 1.0E+04 copies/mL (20 total replicates per level). Above 1.0E+04 copies/mL, one replicate per lot was tested.

For each mutation class of the cobas EGFR Test, the linear range is indicated in Table 26 and the corresponding graphs for one lot are shown in Figure 8 through Figure 14.

Table 26 Linear range of the cobas EGFR Test with K2 EDTA plasma

EGFR Exon	EGFR Mutation	Target Nucleic Acid Sequence	Linear Range (copies/mL)
18	G719A	2156G>C	50 - 1E+04
19	Exon 19 Deletion	2235_2249del15	10 - 1E+05
20	S768I	2303G>T	10 - 1E+05
20	T790M	2369C>T	50 - 1E+05
20	Exon 20 Insertion	2307_2308ins9GCCAGCGTG	10 - 1E+05
21	L858R	2573T>G	10 - 1E+05
21	L861Q	2582T>A	10 - 1E+05


Figure 8 Linearity of mutant DNA in K2 EDTA Plasma:
G719A cell line DNA

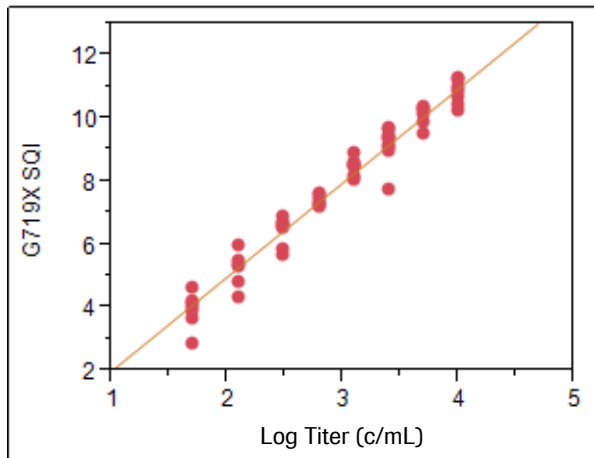

$$\text{SQI} = -0.987 + 2.986 \times \text{Log Copies per mL}$$

$$R^2 = 0.968$$


Figure 9 Linearity of mutant DNA in K2 EDTA Plasma:
Ex19 Del cell line DNA

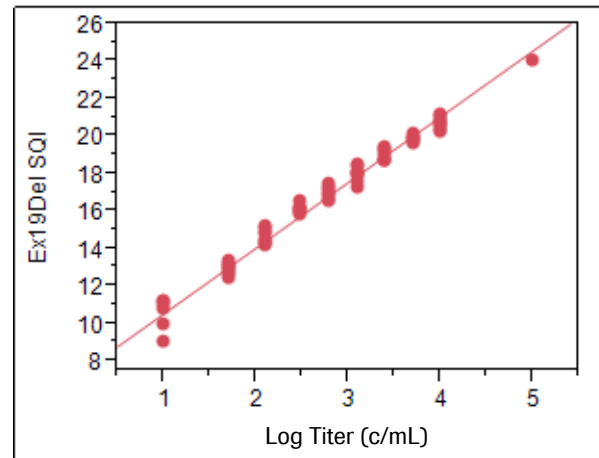

$$\text{SQI} = 7.042 + 3.507 \times \text{Log Copies per mL}$$

$$R^2 = 0.981$$


Figure 10 Linearity of mutant DNA in K2 EDTA Plasma:
S768I cell line DNA

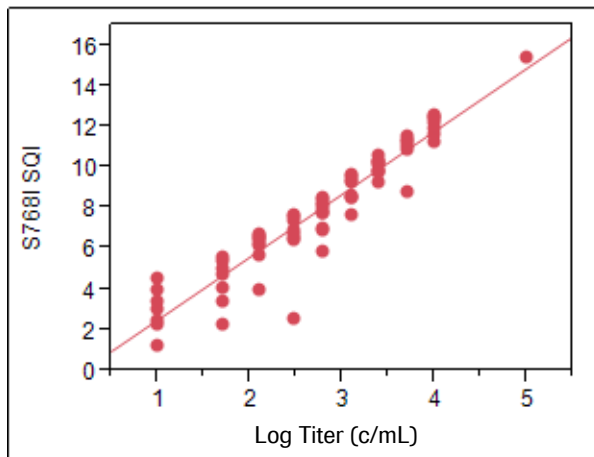

$$\text{SQI} = -0.578 + 3.093 \times \text{Log Copies per mL}$$

$$R^2 = 0.912$$


Figure 11 Linearity of mutant DNA in K2 EDTA Plasma:
T790M cell line DNA

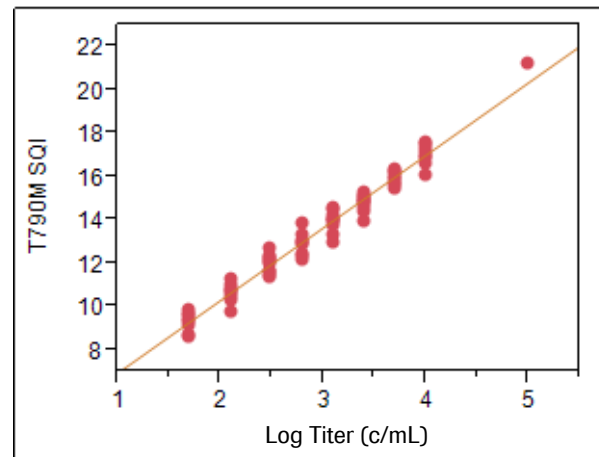

$$\text{SQI} = 3.593 + 3.352 \times \text{Log Copies per mL}$$

$$R^2 = 0.973$$


**Figure 12 Linearity of mutant DNA in K2 EDTA Plasma:
Ex20Ins cell line DNA**

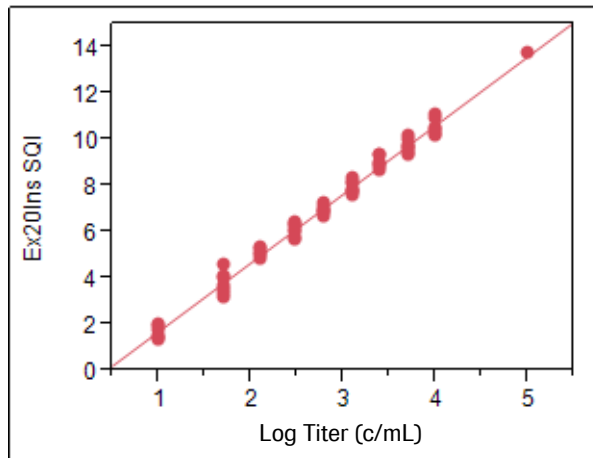

$$\text{SQI} = -1.268 + 2.973 \times \text{Log Copies per mL}$$

$$R^2 = 0.990$$


**Figure 13 Linearity of mutant DNA in K2 EDTA Plasma:
L858R cell line DNA**

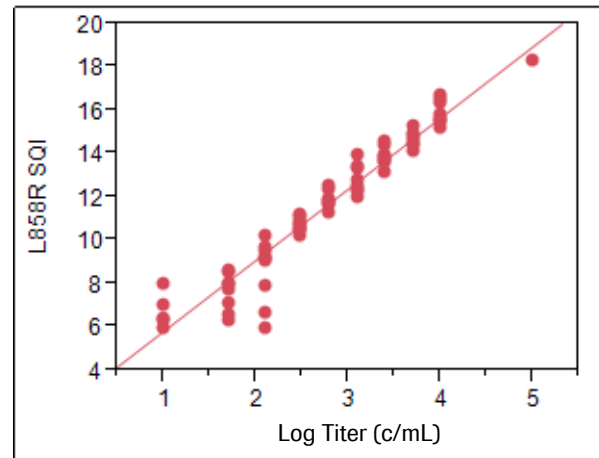

$$\text{SQI} = 2.543 + 3.283 \times \text{Log Copies per mL}$$

$$R^2 = 0.933$$

**Figure 14 Linearity of mutant DNA in K2 EDTA Plasma:
L861Q cell line DNA**

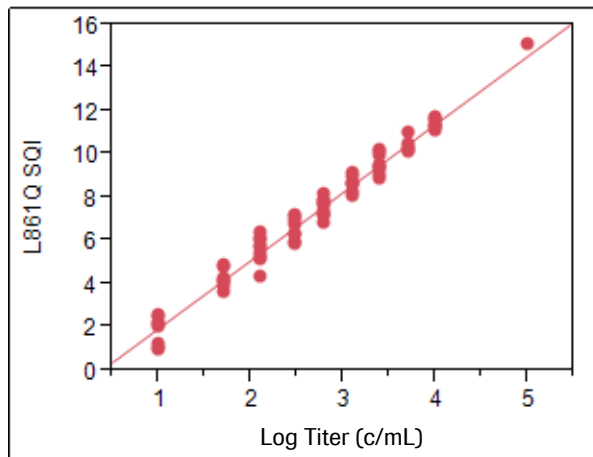

$$\text{SQI} = -1.177 + 3.149 \times \text{Log Copies per mL}$$

$$R^2 = 0.980$$

Roche cfDNA plasma

The linear range with Roche cfDNA plasma was verified using a dilution series of at least 6 panel members spanning the linear range established with K2 EDTA plasma samples (Table 26). Panel members were prepared by diluting sheared cell line DNA containing each of the predominant mutations into EGFR wild-type, healthy-donor Roche cfDNA plasma. The evaluation was performed according to CLSI Guideline EP06-A.²⁴ Four replicates per panel member for each of 2 lots were tested at concentrations up to 1.0E+04 copies/mL (8 total replicates per level). Above 1.0E+04 copies/mL, 2 replicates per lot were tested (4 total replicates per level).

Repeatability

Repeatability of the cobas EGFR Test was assessed using a panel of twelve samples composed of dilutions of EGFR Mutant cell line DNA diluted in healthy donor K2 EDTA plasma samples. The predominant mutation for each class reported by the test were co-diluted into eleven samples and assessed at 3x each mutation's respective LOD (in copies/mL), 1.0E+03 copies/mL, and 5.0E+04 copies/mL. In addition one wild-type sample was tested. Each of the twelve samples was tested in duplicate by two operators, using two different reagent lots over 4 days across two cobas® z 480 analyzers (N = 32 per sample). The cobas EGFR Test had a correct call rate of 99.2% (381/384).

Table 27 lists the mean SQI and the SQI SD from the repeatability study. All 32 replicates for the wild-type sample yielded the expected 'No Mutation Detected' result.

Table 27 Mean SQI and the SQI SD from the repeatability study

EGFR Exon	EGFR Mutation	Target Nucleic Acid Sequence	Concentration (copies/mL)	Mean SQI	SD SQI (n = 32)
18	G719A	2156G>C	3.00E+02	4.53	0.41
			1.00E+03	6.86	0.38
			5.00E+04	11.81	0.67
19	Ex19Del	2235_2249del15	7.50E+01	13.42	0.46
			1.00E+03	16.85	0.42
			5.00E+04	22.31	0.55
20	S768I	2303G>T	6.00E+01	5.99	0.45
			1.00E+03	8.49	0.43
			5.00E+04	14.13	0.43
20	T790M	2369C>T	7.50E+01	9.00	1.03
			1.00E+03	13.28	0.43
			5.00E+04	19.52	0.57
20	Ex20Ins	2307_2308ins9GCCAGCGTG	2.40E+02	4.92	0.43
			1.00E+03	6.77	0.40
			5.00E+04	12.61	0.60
21	L858R	2573T>G	1.20E+02	9.81	0.47
			1.00E+03	12.91	0.28
			5.00E+04	17.21	0.81
21	L861Q	2582T>A	4.50E+01	3.58	0.73
			1.00E+03	7.91	0.45
			5.00E+04	10.06	0.60
EGFR wild type			0	NMD	NMD

"NMD" = No Mutation Detected

Clinical performance evaluation

Clinical reproducibility with K2 EDTA plasma

A study was performed to assess the reproducibility of the cobas EGFR Test across 3 testing sites (2 external and 1 internal, 2 operators per site), 3 reagent lots, and 3 non-consecutive testing days, with a nine-member panel of contrived samples consisting of cell-line DNA diluted in NSCLC plasma. Mutations including one exon 18 G719X mutation, one exon 19 deletion mutation, two exon 20 T790M mutations, one exon 20 insertion mutation, one exon 21 L858R mutation, and one exon 21 L861Q mutation, were represented in four contrived samples as summarized in Table 28. Each contrived sample was prepared at two levels: approximately 100 copies/mL and 300 copies/mL. These contrived samples were built into eight separate panel members along with a wild-type control to make the nine-member panel.

Table 28 Contrived sample mutation combinations

Cell-Line DNA Combination 1	Cell-Line DNA Combination 2	Cell-Line DNA Combination 3	Cell-Line DNA Combination 4
Exon 19 Del	L858R	S768I	L861Q
T790M	T790M	G719A	Exon20 ins

Overall 37 runs were performed with 36 valid runs and one invalid run. A total of 648 panels (or 1224 mutations) were tested, of which 646 panels (or 1220 mutations) had valid results. There were no results of “Mutation Detected” in 72 valid tests of the wild-type panel member, producing 100% agreement. Agreements vary for the mutation members: eight achieved 100% agreement, five > 97%, and one mutation (G719X) demonstrated a lower agreement at approximately 90%. Results for the overall agreement by mutations are presented in Table 29. The coefficient of variation (CV) was ≤ 12.8% in all mutant panel members. For the internal and Mutant controls, the overall CV was ≤ 1.5%. The CV was ≤ 0.89% between lots and ≤ 1.47% within-lot.

Table 29 Overall estimates of agreement by mutation member in reproducibility study

Mutation Member	Number of Valid Tests	Agreement N	Agreement % (95% CI) ^a
Wild Type - NA	72	72	100 (95.0, 100.0)
Exon 18 G719A - 100 Copies/mL	72	65	90.3 (81.0, 96.0) ^b
Exon 19 Deletion (2235_2249del15) - 100 Copies/mL	72	72	100 (95.0, 100.0)
Exon 20 Insertion (2307_2308ins9) - 100 Copies/mL	72	72	100 (95.0, 100.0)
Exon 20 S768I - 100 Copies/mL	72	72	100 (95.0, 100.0)
Exon 20 T790M - 100 Copies/mL	143	139	97.2 (93.0, 99.2)
Exon 21 L858R - 100 Copies/mL	71	70	98.6 (92.4, 100.0)
Exon 21 L861Q - 100 Copies/mL	72	72	100 (95.0, 100.0)
Exon 18 G719A - 300 Copies/mL	71	70	98.6 (92.4, 100.0)
Exon 19 Deletion (2235_2249del15) - 300 Copies/mL	72	72	100 (95.0, 100.0)
Exon 20 Insertion (2307_2308ins9) - 300 Copies/mL	72	72	100 (95.0, 100.0)
Exon 20 S768I - 300 Copies/mL	71	71	100 (94.9, 100.0)
Exon 20 T790M - 300 Copies/mL	144	142	98.6 (95.1, 99.8)
Exon 21 L858R - 300 Copies/mL	72	71	98.6 (92.5, 100.0)
Exon 21 L861Q - 300 Copies/mL	72	72	100 (95.0, 100.0)

^a 95% CI = 95% exact binomial confidence interval.

^b Lower agreement for this sample was due primarily to multiple missed calls (n = 6/24 replicates combined) occurring primarily at one of three sites.

Note: Results were in agreement when a Mutant Type panel member had a valid result of "Mutation Detected" or when wild-type panel member had a valid result of "No Mutation Detected".

Note: The samples used in this study consisted of cell line DNA mechanically sheared to an average size of 220bp and had a WT DNA background of approximately 12,000 copies/mL.

Clinical reproducibility with Roche cfDNA plasma

A study was performed to assess the reproducibility of the cobas EGFR Test across 3 testing sites (2 external and 1 internal, 2 operators per site), one reagent lot, and 3 non-consecutive testing days, with three nine-member panels of contrived samples consisting of cell-line DNA diluted in three unique pools of healthy donor plasma. The samples in each pool were collected with a unique lot of Roche cfDNA tubes. Two of the plasma panels were tested at each site. Mutations including one exon 18 G719X mutation, one exon 19 deletion mutation, one exon 20 T790M mutation, one exon 20 insertion mutation, one exon 21 L858R mutation, and one exon 21 L861Q mutation, were represented in four contrived samples as summarized in Table 30. Each contrived sample was prepared at two levels: approximately 100 copies/mL and 300 copies/mL. These contrived samples were built into eight separate panel members along with a wild-type control to make the nine-member panel.

Table 30 Contrived sample mutation combinations

Cell-Line DNA Combination 1	Cell-Line DNA Combination 2	Cell-Line DNA Combination 3	Cell-Line DNA Combination 4
Exon 19 Del	S768I	T790M	L858R
Exon 20 Ins	G719A	L861Q	n/a

Overall 36 runs were performed and all were valid. A total of 648 panels were tested, of which 646 panels (or 1220 mutations) had valid results. There was one result of “Mutation Detected” in 72 valid tests of the wild-type panel member, producing 98.6% agreement. Agreements vary for the mutation members: thirteen achieved 100% agreement, one > 98%. Results for the overall agreement by mutations are presented in Table 31. The coefficient of variation (CV) was ≤ 13.7% in all mutant panel members. For the internal and Mutant controls, the overall CV was ≤ 1.3%.

Table 31 Overall estimates of agreement by mutation member in reproducibility study

Mutation Member	Number of Valid Tests	Agreement N	Agreement % (95% CI) ^a
Wild Type - NA	72	71	98.6 (92.5, 100.0)
Exon 18 G719A - 100 Copies/mL	72	71	98.6 (92.5, 100.0)
Exon 19 Deletion (2235_2249del15) - 100 Copies/mL	72	72	100 (95.0, 100.0)
Exon 20 Insertion (2307_2308ins9) - 100 Copies/mL	72	72	100 (95.0, 100.0)
Exon 20 S768I - 100 Copies/mL	72	72	100 (95.0, 100.0)
Exon 20 T790M - 100 Copies/mL	72	72	100 (95.0, 100.0)
Exon 21 L858R - 100 Copies/mL	72	72	100 (95.0, 100.0)
Exon 21 L861Q - 100 Copies/mL	72	72	100 (95.0, 100.0)
Exon 18 G719A - 300 Copies/mL	72	72	100 (95.0, 100.0)
Exon 19 Deletion (2235_2249del15) - 300 Copies/mL	71	71	100 (94.9, 100.0)
Exon 20 Insertion (2307_2308ins9) - 300 Copies/mL	71	71	100 (94.9, 100.0)
Exon 20 S768I - 300 Copies/mL	72	72	100 (95.0, 100.0)
Exon 20 T790M - 300 Copies/mL	71	71	100 (94.9, 100.0)
Exon 21 L858R - 300 Copies/mL	72	72	100 (95.0, 100.0)
Exon 21 L861Q - 300 Copies/mL	71	71	100 (94.9, 100.0)

^a 95% CI = 95% exact binomial confidence interval.

Note: Results were in agreement when a Mutant Type panel member had a valid result of “Mutation Detected” or when the wild-type panel member had a valid result of “No Mutation Detected”.

Limit of Detection (LOD) using NSCLC plasma samples

A study was performed to confirm the LOD with K2 EDTA NSCLC plasma samples for three exon 19 deletions, one L858R mutation, and one T790M mutation using the cobas EGFR Test across three testing sites (two external and one internal, two operators per site), three reagent lots, and two non-consecutive testing days, with an 11-member panel of NSCLC plasma samples (five mutations each with two levels: 1 × LOD and 2 × LOD; plus WT). Overall 12 runs were performed (two replicates per run), and all runs were valid. A total of 264 tests were performed with the 11 panel members, of which 262 (99.2%) tests were valid. “Mutation Detected” results were not observed in 23 valid tests of the wild-type panel member, producing 100% agreement. The percentage agreement for Exon 20 T790M-1 × LOD is 95.8%; and 100% for all other mutant panel members. The agreement estimates by panel member are summarized in Table 32. The coefficient of variation (CV) was < 7.0% in all mutant panel members.

Table 32 Agreement estimates by panel member

Panel Member	Number of Valid Tests	Agreement N	Agreement % (95% CI) ^a
Wild Type - NA	23	23	100 (85.2, 100.0)
Exon 19 Deletion 1 - 1 × LOD	24	24	100 (85.8, 100.0)
Exon 19 Deletion 1 - 2 × LOD	24	24	100 (85.8, 100.0)
Exon 19 Deletion 2 - 1 × LOD	23	23	100 (85.2, 100.0)
Exon 19 Deletion 2 - 2 × LOD	24	24	100 (85.8, 100.0)
Exon 19 Deletion 3 - 1 × LOD	24	24	100 (85.8, 100.0)
Exon 19 Deletion 3 - 2 × LOD	24	24	100 (85.8, 100.0)
Exon 20 T790M - 1 × LOD	24	23	95.8 (78.9, 99.9)
Exon 20 T790M - 2 × LOD	24	24	100 (85.8, 100.0)
Exon 21 L858R - 1 × LOD	24	24	100 (85.8, 100.0)
Exon 21 L858R - 2 × LOD	24	24	100 (85.8, 100.0)

^a 95% CI = 95% exact binomial confidence interval.

Note: Results are included as agreement when a valid test of Mutant Type panel member has a result of Mutation Detected or when a valid test of wild-type panel member has a result of 'No Mutation Detected'.

Note: Clinical samples used in this study had a WT DNA background of approximately 24,000 copies/mL.

Correlation of Roche cfDNA plasma to K2 EDTA plasma

The performance of the cobas EGFR test with K2 EDTA plasma and Roche cfDNA plasma was compared by testing a sample panel that included paired draws from 34 EGFR wild-type NSCLC patients, 17 EGFR mutation positive NSCLC patients, and 20 healthy donors. The healthy donor draws were used to construct surrogate samples consisting of sheared cell line DNA containing the predominant mutations reported by the cobas EGFR test spiked into whole blood drawn into K2 EDTA and Roche cfDNA tubes. The spike level for the sheared cell line DNA in the surrogate samples was approximately 1.5 × LOD for each mutation as determined with K2 EDTA plasma (Table 24). The mutation status was confirmed for each NSCLC patient using an NGS method. Each sample was tested with one lot of cobas EGFR Test reagents. All samples yielded valid results and the comparison results are shown in Table 33.

Table 33 Agreement analysis between K2 EDTA plasma and plasma derived from the Roche cfDNA tube

		K2 EDTA Tube		Total
		MD	NMD	
Roche Cell-Free DNA Tube	MD	37	0	37
	NMD	0	34	34
	Total	37	34	71

Positive Agreement (%): 95% CI	100% 90.5% - 100%
Negative Agreement (%): 95% CI	100% 89.7% - 100%
Overall Agreement (%): 95% CI	100% 94.5% - 100%

Where: MD = Mutation Detected and NMD = No Mutation Detected

Concordance between paired samples for K2 EDTA plasma and plasma derived from the Roche Cell-Free DNA Collection Tubes was 100%. No discordant results were observed.

In plasma samples from the study, the **cobas** EGFR Test detected the following mutations in exon 18, 19, 20 and 21 of the EGFR gene listed in Table 34. Unless otherwise noted, the mutations were observed in NSCLC samples.

Table 34 Mutations observed in Correlation of Roche cfDNA plasma to K2 EDTA plasma

Exon	Mutation Sequence	AA Change	COSMIC ID ¹⁴
18	2156G>C*	G719A	6239
	2155G>A [§]	G719S	6252
19	2235_2249del15 ⁺	E746_A750delELREA	6223
	2236_2250del15 [§]	E746_A750delELREA	6225
	2219_2236dup TTCCCGTCGCTATCAAGG [§]	K745_E746insVPVAIK	6963938
	2237_2248del12 [§]	E746_E749delELRE	Not Found
	2237_2251del15 [§]	E746_T751>A	12678
	2239_2240TT>CC [§]	L747P	24267
	2251A>C [§]	T751P	Not Found
20	2369C>T ⁺	T790M	6240
	2303G>T ⁺	S768I	6241
	2307_2308insGCCAGCGTG*	V769_D770insASV	12376
21	2573T>G ⁺	L858R	6224
	2582T>A*	L861Q	6213

* Observed only in surrogate sample

⁺ Observed in surrogate sample and NSCLC sample

[§] Observed only in NSCLC sample

Correlation to reference method using Phase III plasma samples from the ASPIRATION cohort

The analytical accuracy of the **cobas** EGFR Test in detecting exon 19 deletion and L858R mutations was assessed by comparing with a validated next generation sequencing (NGS) platform using K2 EDTA plasma samples from patients with advanced NSCLC from one or more of the following studies (ASPIRATION Cohort): Genentech clinical studies G027821 (MetMab) and G027761 (MetLung) along with Roche clinical study ML25637 (ASPIRATION).

One hundred and twenty-eight plasma samples with a volume of 2 mL and with valid paired results from both the **cobas** EGFR Test in plasma and a NGS method using plasma samples were included in the agreement analysis for the EGFR exon 19 deletion or L858R mutations. A total of 32 samples had MD and 95 had NMD results by the NGS method. The PPA between the **cobas** EGFR Test in plasma and NGS in plasma was 87.5% (95% CI: 71.9%, 95.0%); the NPA between the **cobas** EGFR Test and NGS was 96.8% (95% CI: 91.1%, 98.9%), as presented in Table 35.

Table 35 Comparison of the cobas EGFR Test in plasma with NGS for the detection of the EGFR exon 19 deletion or L858R mutations

Measure of Agreement	Percent Agreement (N)	95% CI
Positive Percent Agreement (PPA)	87.5% (28/32)	71.9%, 95.0%
Negative Percent Agreement (NPA)	96.8% (92/95)	91.1%, 98.9%

Correlation between plasma and tissue samples by the cobas EGFR Test for the detection of exon 19 deletion and L858R mutations using Phase III samples from ENSURE

The ENSURE study (YO25121) was a multicenter, open label, randomized Phase III study to evaluate the efficacy and safety of TARCEVA® (erlotinib) versus gemcitabine/cisplatin as the first-line treatment for stage IIIB/IV non-small cell lung cancer (NSCLC) patients with exon 19 deletion or L858R mutations in the tyrosine kinase domain of epidermal growth receptor (EGFR) in their tumors. A total of 647 patients were screened, 601 patients had valid tissue EGFR results for exon 19 deletion and L858R Mutation from the **cobas** EGFR Test, and 217 patients were randomized in the study.

Five hundred and seventeen patients (86.0%, 517/601) had matched K2 EDTA plasma and tissue samples and 441 patients had a plasma sample volume ≥ 2.0 mL, i.e. the sample volume for which the **cobas** EGFR Test in plasma was validated.

The correlation of plasma and tissue samples by the **cobas** EGFR Test for detection of the exon 19 deletion and L858R mutation was evaluated both separately and in aggregate. A total of 431 samples with paired valid results from both tissue and plasma samples by **cobas** EGFR Test were included in the agreement analysis. The positive percent agreement (PPA) between plasma and tissue sample was 76.7% (95% CI: 70.5% to 81.9%), the negative percent agreement (NPA) was 98.2% (95% CI: 95.4% to 99.3%), for the detection of exon 19 deletion and L858R mutation in aggregate as presented in Table 36. The PPA, NPA and OPA for detection of exon 19 deletion and L858R mutation separately are also presented in Table 36.

Table 36 Agreement between plasma samples and tissue samples by cobas EGFR Test in the detection of Exon 19 deletion and L858R mutation

Mutation	Measure of Agreement	Percent Agreement (N)	95% CI
Aggregate	Positive Percent Agreement (PPA)	76.7% (161/210)	70.5%, 81.9%
	Negative Percent Agreement (NPA)	98.2% (217/221)	95.4%, 99.3%
	Overall Percent Agreement (OPA)	87.7% (378/431)	84.2%, 90.5%
Exon 19 Deletion	Positive Percent Agreement (PPA)	80.8% (97/120)	72.9%, 86.9%
	Negative Percent Agreement (NPA)	98.7% (307/311)	96.7%, 99.5%
	Overall Percent Agreement (OPA)	93.7% (404/431)	91.0%, 95.7%
L858R	Positive Percent Agreement (PPA)	67.8% (61/90)	57.6%, 76.5%
	Negative Percent Agreement (NPA)	99.1% (338/341)	97.4%, 99.7%
	Overall Percent Agreement (OPA)	92.6% (399/431)	89.7%, 94.7%

Note: PPA and NPA calculated using tissue as the reference.

Positive predictive value (PPV) and negative predictive value (NPV) for detection of exon 19 deletion and L858R mutations in aggregate were also calculated using the bootstrap method based on the different population tissue prevalence (Table 37). As expected, the PPV increases and NPV decreases as the EGFR mutation prevalence increases. For a Caucasian patient population, which assumes 10-15% tissue EGFR mutation prevalence, the PPV ranges from 82.8% to 88.6% while NPV ranges from 96.0% to 97.4%. The PPV ranges from 94.8% to 97.8% while NPV ranges from 80.8% to 90.9% if based on the prevalence in an Asian population, assuming 30-50% tissue EGFR mutation prevalence.

Table 37 Estimated predictive values of the cobas EGFR Test in tissue and cobas EGFR Test in plasma (patients with plasma sample volumes ≥ 2.0 mL) based on differing tissue EGFR mutation prevalence

Assumed EGFR Prevalence Based on Tissue Samples	Positive Predictive Value (PPV)	Negative Predictive Value (NPV)
10%	82.8% (71.3%, 93.7%)	97.4% (96.2%, 98.7%)
15%	88.6% (79.7%, 96.9%)	96.0% (94.3%, 97.6%)
20%	91.6% (85.0%, 97.8%)	94.4% (92.3%, 96.3%)
30%	94.8% (90.0%, 98.6%)	90.9% (88.4%, 93.4%)
40%	96.8% (93.0%, 99.4%)	86.4% (83.3%, 89.4%)
50%	97.8% (95.0%, 100.0%)	80.8% (77.4%, 84.8%)

Note: The 95% CIs were calculated from the bootstrap method.

Note: The result of 79 samples with a volume < 2.0 mL were treated as invalid in this analysis.

Note: PPV and NPV calculated using plasma as the reference.

Correlation to reference method using Phase II samples from AURA2

The clinical performance of the cobas EGFR Test was assessed by comparing it with a validated next generation sequencing (NGS) platform using K2 EDTA plasma samples from patients with advanced NSCLC who were screened in the Phase II AURA2 trial with TAGRISSO®.²³

Of the 383 eligible patients, 344 patients had a plasma sample available and were tested by the cobas EGFR Test, with 342 valid results and two invalid results. Of a total of 344 plasma sample tested by the cobas EGFR Test, 322 (93.6%) were also tested by an NGS method and 22 did not have enough plasma volume remaining to be tested by NGS.

The analytical accuracy of the cobas EGFR Test compared with the reference method, NGS, for detection of the T790M mutation in plasma samples was evaluated. A total of 320 samples with valid paired results from both cobas EGFR Test and NGS results were included in the agreement analysis. The positive percent agreement (PPA) between the cobas EGFR Test and NGS was 91.5% (95% CI: 85.7% to 95.1%), the negative percent agreement (NPA) was 91.1% (95% CI: 86.0% to 94.4%), for the detection of the T790M mutation as presented in Table 38.

Table 38 Comparison of the cobas EGFR Test in plasma with NGS for the detection of the EGFR T790M mutation

Measure of Agreement	Percent Agreement (N)	95% CI
Positive Percent Agreement (PPA)	91.5% (129/141)	85.7%, 95.1%
Negative Percent Agreement (NPA)	91.1% (163/179)	86.0%, 94.4%

In K2 EDTA plasma samples from the AURA2 trial, the cobas EGFR Test detected mutations in exon 18, 19, 20 and 21 of the EGFR gene as listed in Table 39.

Table 39 Mutations detected by the cobas EGFR Test in the AURA 2 cohort

Exon	Mutation Sequence	AA Change	COSMIC ID ¹⁴
18	2156G>C	G719A	6239
	2155G>A	G719S	6252
	2155G>T	G719C	6253
19	2235_2249del15	E746_A750delELREA	6223
	2236_2250del15	E746_A750delELREA	6225
	2236_2256>ATC	E746_S752>I	133190
	2237_2251del15	E746_T751>A	12678
	2237_2255>T	E746_S752>V	12384
	2237_2258>TATC	E746_P753>VS	Not Found
	2238_2248>GC	L747_A750>P	12422
	2239_2247delTTAAGAGAA	L747_E749delLRE	6218
	2239_2248TTAAGAGAAG>C	L747_A750>P	12382
	2239_2251>C	L747_T751>P	12383
	2239_2256>CAG	L747_S752>Q	Not Found
	2239_2256del18	L747_S752delLREATS	6255
	2239_2258>CA	L747_P753>Q	12387
	2239_2264>GCCAA	L747_A755>AN	85891
	2240_2251del12	L747_T751>S	6210
	2240_2254del15	L747_T751delLREAT	12369
	2240_2257del18	L747_P753>S	12370
	2240_2264>CGAGAGA	L747_A755>SRD	Not Found
2253_2276del24	S752_I759delSPKANKEI	13556	
20	2369C>T	T790M	6240
	2303G>T	S768I	6241
21	2573T>G	L858R	6224
	2573_2574TG>GT	L858R	12429
	2582T>A	L861Q	6213

Correlation between plasma and tissue samples for the detection of T790M using Phase II samples from AURA2

The AURA2 clinical trial²³ was a Phase II, open-label, single-arm study, assessing the safety and efficacy of TAGRISSO® (osimertinib) as a second or ≥ third-line therapy in patients with advanced NSCLC, who had progressed following prior therapy with an approved EGFR TKI agent and were T790M positive as determined by the cobas EGFR Test. A total of 472 patients were screened, 383 patients had a tissue sample tested and 371 patients had a valid tissue EGFR result for the T790M mutation from the cobas EGFR Test, of which 233 patients were T790M positive and 210 patients were randomized in the study.

Of the 383 eligible patients, 344 patients had K2 EDTA plasma samples. A total of 334 samples with paired valid results from both tissue and plasma samples by the **cobas** EGFR Test were included in the analysis. The positive percent agreement (PPA) between plasma and tissue samples was 58.7% (95% CI: 52.2%, 65.0%) and the negative percent agreement (NPA) was 80.2% (95% CI: 71.8%, 86.5%) for the detection of the T790M mutation. The positive predictive value (PPV) was 85.6% (95% CI: 79.2%, 90.3%) and the negative predictive value (NPV) was 49.2% (95% CI: 42.0%, 56.4%) for the detection of the T790M mutation as presented in Table 40.

The PPV shown in Table 40 was impacted by the 22 samples which were T790M negative by the **cobas** EGFR Test in tissue and T790M positive by the **cobas** EGFR Test in plasma. Eighteen samples were confirmed as T790M positive by NGS in plasma and one sample did not have enough volume for NGS testing. Only three were determined to be T790M negative by NGS.

Table 40 Agreement between plasma samples and tissue samples by the cobas EGFR Test in the detection of the T790M mutation

Mutation	Measure of Agreement	Percent Agreement (N)	95% CI
T790M	Positive Percent Agreement (PPA)	58.7% (131/223)	52.2%, 65.0%
	Negative Percent Agreement (NPA)	80.2% (89/111)	71.8%, 86.5%
	Overall Percent Agreement (OPA)	65.9% (220/334)	60.6%, 70.8%
	Positive Predictive Value (PPV)	85.6% (131/153)	79.2%, 90.3%
	Negative Predictive Value (NPV)	49.2% (89/181)	42.0%, 56.4%

Note: PPA and NPA calculated using tissue as the reference.

Note: PPV and NPV calculated using plasma as the reference.


The agreement between plasma and tissue samples in the detection of the T790M resistance mutation is lower than for activating mutations. The PPA can be affected by tissue heterogeneity: unlike the activating mutations L858R and exon 19 deletions, T790M may be present in a small percentage of tumor cells as it is generally an acquired mutation; therefore, T790M cfDNA may only be present in very low concentration in plasma and below the level of detection. The NPA can also be affected by tumor heterogeneity: because the T790M mutation may not be present in all tumor cells, a tissue biopsy may be taken from a tumor in which the T790M mutation is not present while other tumor sites may be T790M-positive.⁷

Clinical outcome data

ENSURE


In the ENSURE trial, of the 217 patients enrolled (i.e., those with an exon 19 deletion or L858R mutation detected in a tissue sample by the **cobas** EGFR Test v1), 214 (98.6%) had a K2 EDTA plasma sample available and 180 patients had a plasma sample volume of 2.0 mL. Of the 180 plasma samples with a volume of 2 mL tested by **cobas** EGFR Test, 137 had a “Mutation Detected” result for an exon 19 deletion or an L858R mutation (68 patients in the erlotinib arm, 69 patients in the chemotherapy arm), 42 had a “No Mutation Detected” result (22 patients in the TARCEVA® arm, 20 patients in the chemotherapy arm), and one sample generated an invalid result. The Kaplan-Meier curves for the investigator assessed PFS are shown in Figure 15 for patients with either an exon 19 deletion or L858R mutation in a plasma sample. The patients in the TARCEVA® arm had a longer PFS compared to patients in the chemotherapy arm and the two curves were well separated over the course of the observation period (p value < 0.001) showing substantial benefit to therapy with TARCEVA® in patients with a detectable EGFR activating mutation in plasma.

Figure 15 Kaplan-Meier Plot of PFS by treatment for patients with mutation detected by the cobas EGFR Test in both plasma and tissue (investigator assessment) (with 2 mL plasma samples)

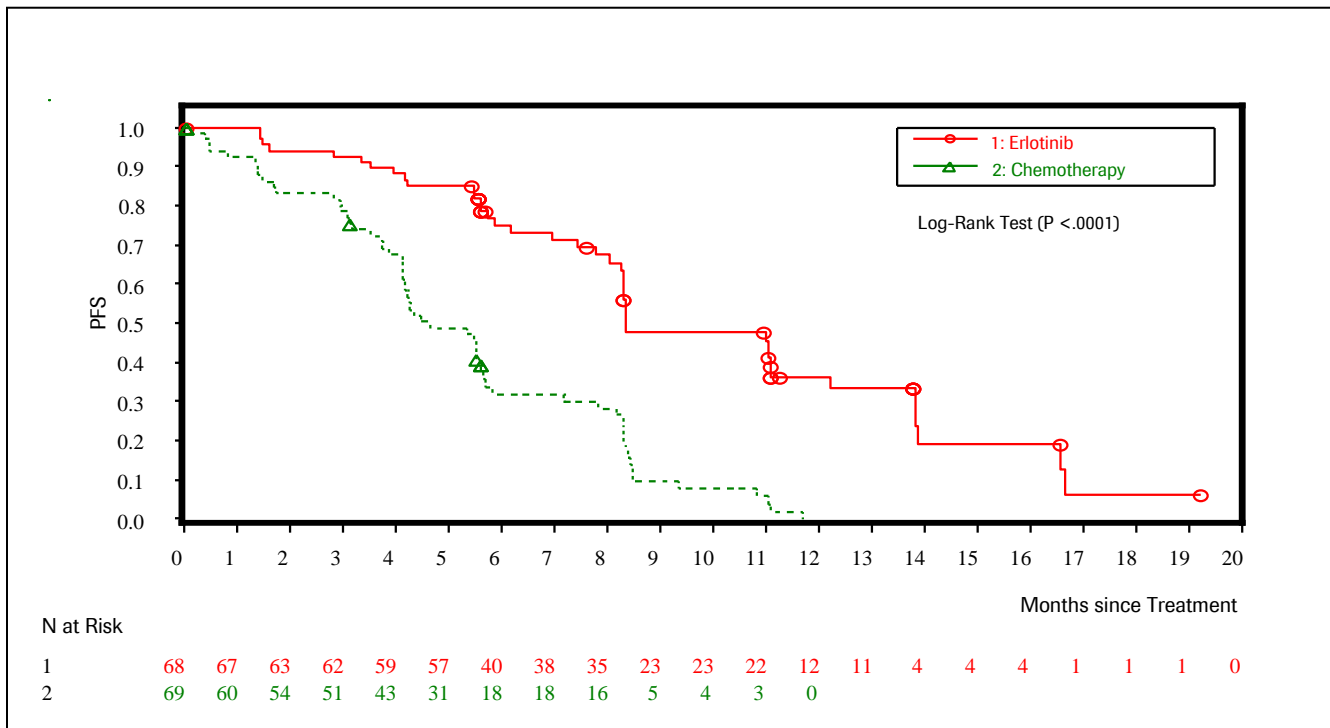

A consistent PFS benefit was observed for all patients who were tissue EGFR mutation positive with plasma sample volumes of 2.0 mL whether they were plasma mutation positive or negative and this benefit was similar to the PFS benefit observed in the overall ENSURE ITT population (HR = 0.33; 95% CI: 0.23, 0.47) as shown in Figure 16 below.

Figure 16 Forest plot for the HRs for PFS by investigator assessment (with 2 mL plasma samples)

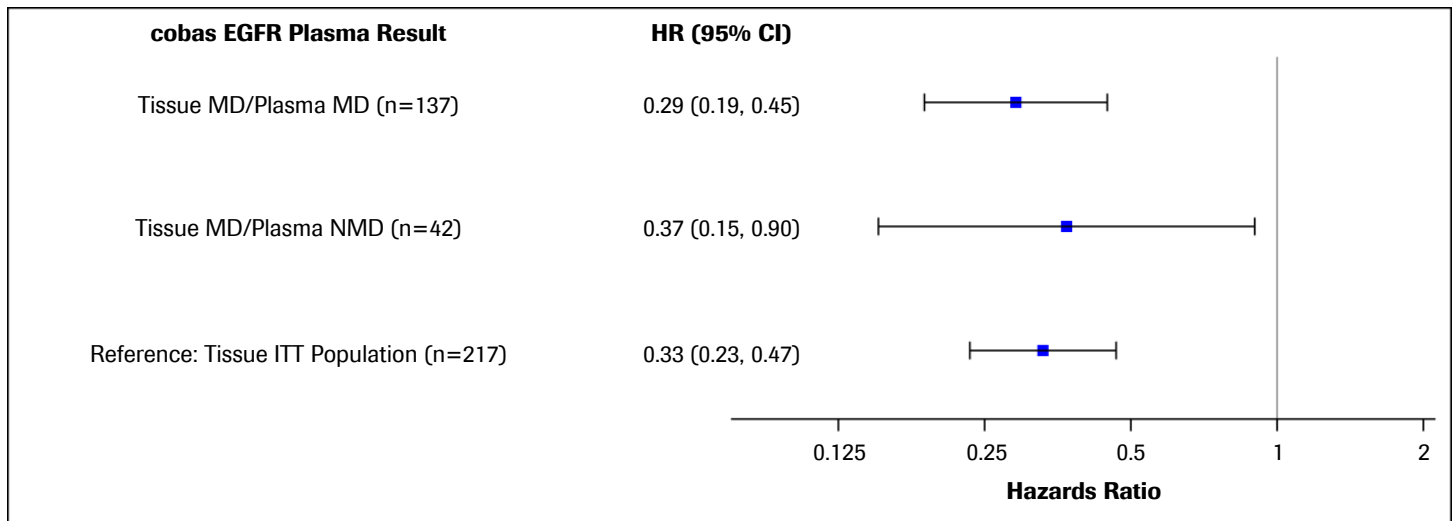

Note: MD = Mutation Detected (exon 19 deletion or L858R); NMD = No Mutation Detected (exon 19 deletion and L858R)

AURA2

The primary efficacy endpoint variable was the objective response rate (ORR) according to RECIST 1.1 by BICR using the evaluable for response analysis set. The ORR was defined as the number (%) of patients with at least one visit and a result of complete response (CR) or partial response (PR) that was confirmed at least four weeks later (i.e., a best objective response [BOR] of CR or PR).

In the tissue Evaluable Response Analysis Set (ERAS) population (T790M+ patients by the cobas EGFR Test in tissue who received at least one dose of TAGRISSO® and had measurable disease at baseline according to BICR), 111 patients were K2 EDTA plasma T790M+ by the cobas EGFR Test (i.e. T790M+ by both the tissue and plasma samples). The ORR for this subset was 64.9% (72/111, 95% CI: 52.1%, 70.4%), which is very similar to the 64.1% observed ORR in the tissue ERAS population.

In the tissue Full Analysis Set (FAS) population (T790M+ patients by the cobas EGFR Test in tissue who received at least one dose of TAGRISSO®), 117 patients were plasma T790M+ by the cobas EGFR Test. The ORR for patients with a T790M+ result by both tissue and plasma samples was 61.5% (72/117, 95% CI: 55.2%, 73.7%), which is also very similar to the 61% observed ORR in the tissue FAS population. The results of these analyses are presented in Table 41. As enrollment in AURA2 was based on positive tissue test results, outcome data for (T790M plasma+, T790M tissue-) patients are not available from this trial.

Table 41 Objective response rate by plasma result among enrolled patients (T790M+ by tissue) from AURA2 study

Population (T790M+ by tissue sample)	Results of cobas EGFR Test from Plasma Sample	N	Number of Patients with Response (ORR) ^a n (%)	ORR (95% CI)
Tissue Full Analysis Set (Tissue FAS)	T790M+(Plasma FAS)	117	72 (61.5%)	(55.2%, 73.7%)
	T790M-	89	53 (59.6%)	(51.3%, 73.0%)
	Overall (Tissue FAS)	210	128 (61.0%)	(57.0%, 70.8%)
Tissue Evaluable Response Analysis Set (Tissue ERAS)	T790M+(Plasma ERAS)	111	72 (64.9%)	(52.1%, 70.4%)
	T790M-	83	52 (62.7%)	(48.6%, 69.8%)
	Overall (Tissue ERAS)	198	127 (64.1%)	(54.0%, 67.6%)

^a Responses include confirmed responses only.


FLAURA

I. Phase III Trial for TAGRISSO® First-Line

A total of 994 patients were screened the FLAURA study¹⁰ 556 patients were randomized into the clinical trial and 438 failed screening. Of the 556 FLAURA randomized patients, 537 were eligible for study analysis. Of the 537 study eligible patients, 276 were randomized by a central cobas EGFR tissue test, of which 254 had a K2 EDTA plasma sample available for testing with 190 positive for cobas EGFR plasma test (pEGFRm+); 261 were randomized by a local tissue test, of which 242 had a plasma sample available for testing with 169 positive for cobas EGFR plasma test (136 cobas tissue EGFR mutation positive (tEGFRm+), 1 cobas tissue EGFR mutation negative (tEGFRm-), and 32 invalid/not tested by cobas tissue test).


For the plasma primary population (tEGFRm+ and pEGFRm+) by the cobas EGFR Test, N = 326, 190 centrally randomized and 136 locally randomized), the HR was 0.41 (95% CI: 0.31, 0.54) and the HR for the FLAURA FAS (tEGFRm+, N = 556) was 0.46 (95% CI: 0.37, 0.58). Therefore, the drug efficacy for plasma primary population is consistent with the FLAURA FAS population. The Kaplan Meier plot for the plasma primary population with either an exon 19 deletion or L858R mutation in a plasma sample is shown in Figure 17.

Figure 17 Kaplan-Meier Plot of PFS by treatment for FLAURA plasma primary population (patients who were cobas tEGFR+ and cobas pEGFR+, n = 326)

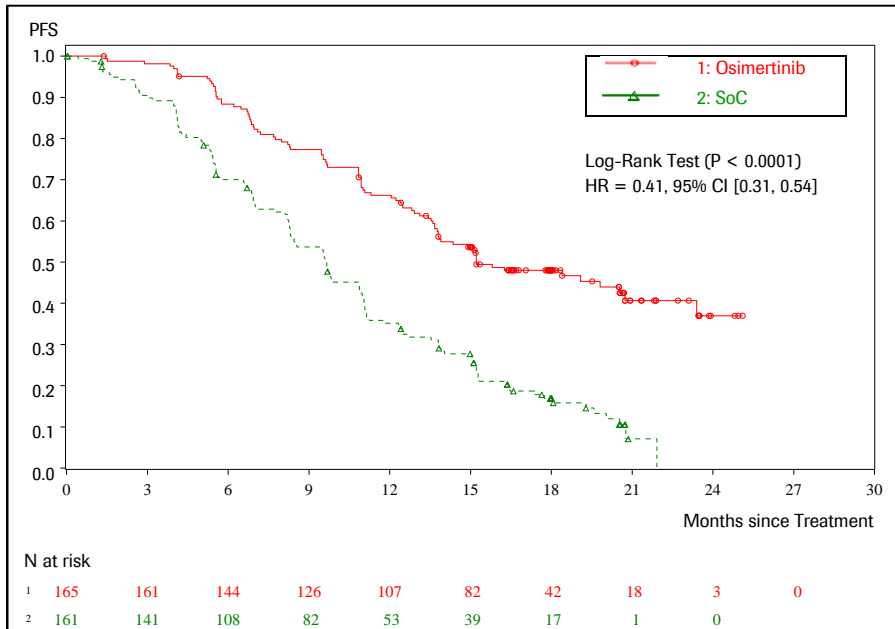

The superiority of TAGRISSO® over SoC was consistent across all plasma positive subgroups defined by local and central cobas tEGFR enrollment status, with HRs ranging from 0.39 to 0.48 and consistent to the HR obtained from the FLAURA FAS population (HR = 0.46) as shown in Figure 18 below.

Figure 18 Forest Plot for the HRs for FLAURA Subgroups Defined by Local and Central cobas EGFR Test Status

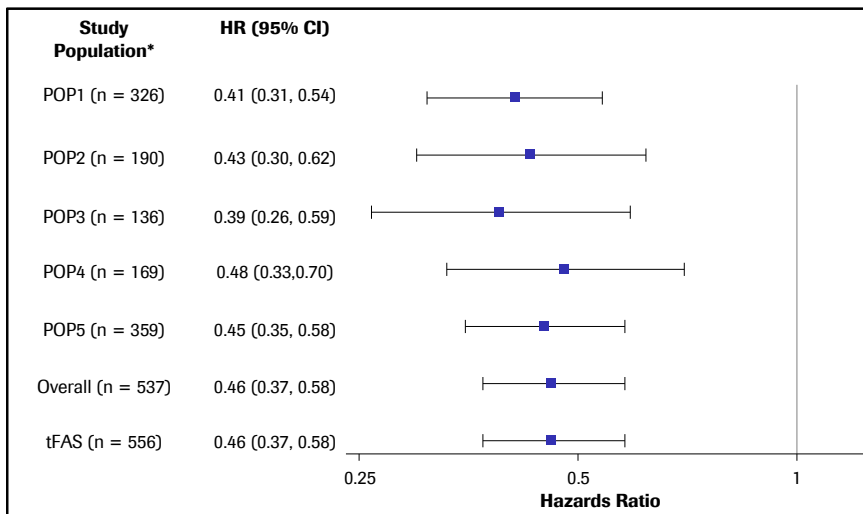

POP = Population (subgroup)

*POP1: All randomized patients with a positive cobas tissue test and cobas plasma test.

POP2: Patients randomized by cobas tissue test and also positive by cobas plasma test.

POP3: Patients randomized by local tissue test and also positive by cobas tissue and plasma test.

POP4: Patients randomized by local tissue test and also positive by cobas plasma test.

POP5: All randomized patients with a positive cobas plasma test.

Overall: All randomized patients excluding 19 China patients.

tFAS: All randomized patients (FLAURA full analysis set).

II. IRESSA® Standard of Care Analysis

A separate analysis was performed on those patients from the standard of care arm (SoC) treated with IRESSA® (gefitinib). Of all IRESSA® treated patients with an investigator-assessed objective response in FLAURA, 105 patients were positive by the cobas plasma test from K2 EDTA samples. The ORR for all cobas plasma positive patients was 71.4% (75/105, 95% CI: 62.2%, 79.2%, POP4 in Table 42).

Of the 105 patients with positive results from the cobas plasma test, 47 patients were randomized by the cobas tissue test (primary efficacy population for cobas plasma test) and 58 patients were randomized by a local test. A total of 36 patients were considered as responders by investigator assessment in the primary efficacy population for cobas plasma test (n = 47), resulting in an ORR of 76.6% (95% CI: 62.8%, 86.4%, POP1 in Table 42).

The ORR was 62.2% (28/45, 95% CI: 47.6%, 74.9%) in locally randomized patients who were positive by both cobas tissue and cobas plasma tests (POP2 in Table 42). The ORR was 69.6% (64/92, 95% CI: 59.5%, 78.0%) in all IRESSA®-treated patients who were both cobas tissue and cobas plasma positive (POP3 in Table 42). A Forest plot of the ORRs for those different patient populations is shown in Figure 19. The results indicate that the treatment effect of IRESSA®, based on the cobas plasma test was maintained in each subpopulation and consistent with the results reported for the original registration study (IFUM) for patients selected for IRESSA®.¹³

Table 42 ORRs for cobas Plasma Positive IRESSA®-Treated Patients in FLAURA

Objective Response	Plasma Positive (pEGFR+) Patients in SoC Arm Treated with IRESSA®				Total
	pEGFR+ Centrally Randomized (cobas tEGFR+)	pEGFR+ Locally Randomized (Local tEGFR+)			
		cobas tEGFR+	cobas tEGFR-	cobas tEGFR Invalid/Not Tested	
No. of Patients	47	45	1	12	105
Response	36	28	1	10	75
Non-Response	11	17	0	2	30
ORR (%), 95% CI)	POP1 = 76.6% (36/ 47: 62.8%, 86.4%)	POP2 = 62.2% (28/ 45: 47.6%, 74.9%)	-	-	POP4 = 71.4% (75/105: 62.2%, 79.2%)
	POP3 = 69.6% (64/ 92: 59.5%, 78.0%)		-	-	-

Note: tEGFR = tissue EGFR; pEGFR = plasma EGFR; CI = (score) Confidence Interval.

POP = population (sub-group)


POP1: ORR for cobas pEGFR+ patients randomized by cobas tissue test (primary efficacy population for cobas plasma test).

POP2: ORR for cobas plasma and tissue positive patients randomized by a local tissue test.

POP3: ORR for all cobas plasma and tissue positive patients.

POP4: ORR for all cobas plasma positive patients.

Figure 19 Forest Plots of ORRs Based on cobas EGFR Test in Plasma for Different Populations

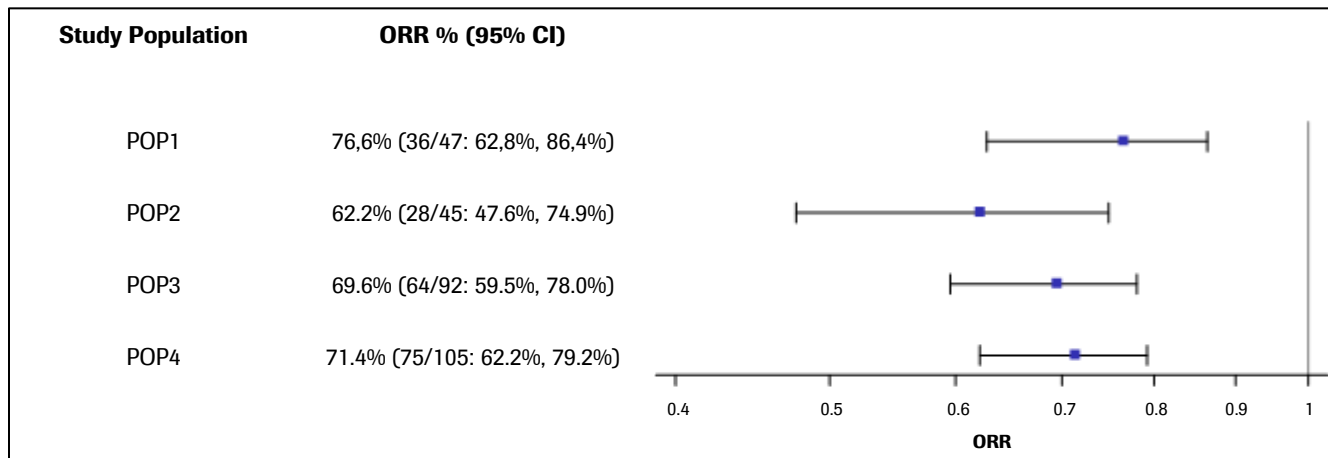

POP = population (sub-group)

POP1: ORR for **cobas** pEGFR+ patients randomized by **cobas** tissue test (primary efficacy population for **cobas** plasma test).

POP2: ORR for **cobas** plasma and tissue positive patients randomized by a local tissue test.

POP3: ORR for all **cobas** plasma and tissue positive patients.

POP4: ORR for all **cobas** plasma positive patients.

Result flags

Explanation of result flags

The source of a flag is indicated in the flag code as outlined in Table 43.

Table 43 Flag source

Flag code starts with	Flag source	Example
M ^a	Multiple or other reasons	M6
R	Result interpretation	R20
Z ^a	Analyzer	Z1

^a Refer to the **cobas®** 4800 System – Operator’s Manual or **cobas®** 4800 System - User Assistance

Table 44 lists all result flags of the system that are user relevant.

Table 44 List of result interpretation flags

Flag Code	Severity	Description	Recommended Action
R797, R807, R817, R827, R837, R842, R847	Error	No target could be detected	Repeat the sample. Refer to the Test procedure section. These flag codes indicate that a negative result occurred for the sample (i.e. sample may have not been added to one or more wells).
R700, R718, R724, R736, R742, R748, R766, R712, R754, R760	Error	Mutant Control could not be detected	Repeat the run. Refer to the Test procedure section. These flag codes indicate that the elbow determination algorithm encountered an error which may occur in the event of an atypical or noisy fluorescence pattern.
R701, R719, R725, R737, R743, R749, R767, R713, R755, R761	Error	Mutant Control could not be detected	Repeat the run. Refer to the Test procedure section. These flag codes indicate that a negative result occurred for the Mutant Control. A Mutant Control DNA may have not been added to one or more wells).
R702, R720, R726, R738, R744, R750, R768, R714, R756, R762	Error	Mutant Control is out of range	Repeat the run. Refer to the Test procedure section. These flag codes indicate that an observed Ct value for the Mutant Control was above the established threshold (i.e. elbow too high). Possible reasons could be: 1. Incorrect preparation of the working Master Mix 2. Pipetting error when adding working Master Mix into a well of the microwell plate 3. Pipetting error when adding Mutant Control into a well of the microwell plate.
R703, R721, R727, R739, R745, R751, R769, R715, R757, R763	Error	Mutant Control is out of range	Repeat the run. Refer to the Test procedure section. These flag codes indicate that an observed Ct value for the Mutant Control was below the established threshold (i.e. elbow too low). This error may occur in the event of DNA contamination.
R772, R778, R780, R784, R786, R788, R794, R776, R790, R792	Error	Negative Control could not be detected	Repeat the run. Refer to the Test procedure section. These flag codes indicate that the elbow determination algorithm encountered an error which may occur in the event of an atypical or noisy fluorescence pattern.





















































Flag Code	Severity	Description	Recommended Action
R773, R779, R781, R785, R787, R789, R795, R777, R791, R793	Error	Negative Control is out of range	Repeat the run. Refer to the Test procedure section. These flag codes indicate that a positive result occurred for the Negative Control (i.e. a contamination event occurred).
R796, R816, R826, R836, R806, R841, R846	Error	No target could be detected	Repeat the sample. Refer to the Test procedure section. These flag codes indicate that the elbow determination algorithm encountered an error which may occur in the event of an atypical or noisy fluorescence pattern.
R799, R819, R829, R839, R809, R844, R849	Error	Result is out of range	Repeat the sample. Refer to the Test procedure section. These flag codes indicate that an atypically low Ct value was observed for the sample.
R800, R820, R830, R840, R810, R845, R850	Error	Result is out of range	Repeat the sample. Refer to the Test procedure section. These flag codes indicate that an atypical relationship between the Mutant Ct value and the Internal Control Ct value was observed for the sample.
R811, R831, R851	Error	Internal Control could not be detected	Repeat the sample. Refer to the Test procedure section. These flag codes indicate that the elbow determination algorithm encountered an error which may occur in the event of an atypical or noisy fluorescence pattern.
R812, R832, R852	Error	Internal Control could not be detected	Repeat the sample. Refer to the Test procedure section. These flag codes indicate that the Internal Control result for the sample was not valid. The absence of a valid Internal Control result suggests: <ol style="list-style-type: none"> 1. Poor quality genomic DNA from the sample 2. Inadequate sample processing 3. The presence of PCR inhibitors in the sample 4. Rare mutations within the regions of the Genomic DNA covered by the Internal Control primers and/or probes 5. Sample DNA may have not been added to one or more wells 6. Other factors.
R813, R834, R853	Error	Internal Control out of range	Repeat the sample. Refer to the Test procedure section. These flag codes indicate that the Internal Control result for the sample was not valid. The absence of a valid Internal Control result suggests: <ol style="list-style-type: none"> 1. Poor quality genomic DNA from the sample 2. Inadequate sample processing 3. The presence of PCR inhibitors in the sample 4. Rare mutations within the regions of the Genomic DNA covered by the Internal Control primers and/or probes 5. Sample DNA may have not been added to one or more wells 6. Other factors.
R814, R835, R854	Error	Internal Control out of range	Repeat the sample. Refer to the Test procedure section. These flag codes indicate that an atypically low Internal Control Ct value was observed for the sample. This error may occur if the PCR mixture is overloaded with concentrated genomic DNA.

Additional information

Symbols

The following symbols are used in labeling for Roche PCR diagnostic products.

Table 45 Symbols used in labeling for Roche PCR diagnostic products

 Age or Date of Birth	 Device not for near-patient testing	 QS IU/PCR	QS IU per PCR reaction, use the QS International Units (IU) per PCR reaction in calculation of the results.
 Ancillary Software	 Device not for self-testing		
 Assigned Range [copies/mL]	 Distributor <i>(Note: The applicable country/region may be designated beneath the symbol)</i>	 SN	Serial number
 Assigned Range [IU/mL]	 Do not re-use	 Site	Site
 EC REP	 Female	 Procedure Standard	Standard Procedure
 Barcode Data Sheet	 For IVD performance evaluation only	 STERILE EO	Sterilized using ethylene oxide
 LOT	 GTIN	 Store in dark	
 Biological risks	 Importer	 Temperature limit	
 REF	 IVD	 TDF	Test Definition File
 CE marking of conformity; this device is in conformity with the applicable requirements for CE marking of an in vitro diagnostic medical device	 LLR	 This way up	
	 Male	 Procedure UltraSensitive	Ultrasensitive Procedure
 Collect Date	 Manufacturer	 UDI	Unique Device Identifier
 Consult instructions for use	 CONTROL -	 ULR	Upper Limit of Assigned Range
 Contains sufficient for <n> tests	 NON STERILE	 Urine Fill Line	Urine Fill Line
 CONTENT	 Patient Name	 Rx Only	US Only: Federal law restricts this device to sale by or on the order of a physician.
 CONTROL	 Patient number	 Use-by date	
 Date of manufacture	 Peel here		
 Device for near-patient testing	 CONTROL +		
 Device for self-testing	 QS copies / PCR		QS copies per PCR reaction, use the QS copies per PCR reaction in calculation of the results.

Technical support

For technical support (assistance) please reach out to your local affiliate:
https://www.roche.com/about/business/roche_worldwide.htm

Manufacturer

Table 46 Manufacturer

Manufactured in the United States



Roche Diagnostics GmbH
Sandhofer Strasse 116
68305 Mannheim, Germany
www.roche.com

Made in USA

Trademarks and patents

See <https://diagnostics.roche.com/us/en/about-us/patents>

Copyright

©2023 Roche Molecular Systems, Inc.

References

1. Sharma S. V., Bell D. W., Settleman J., Haber D. A. Epidermal growth factor receptor mutations in lung cancer. *Nat Rev Cancer*. 2007;7(3):169-81.
2. Pao W., Chmielecki J. Rational, biologically based treatment of EGFR-mutant non-small-cell lung cancer. *Nat Rev Cancer*. 2010;10(11):760-774.
3. Zhou C., Wu Y. L., Chen G., Feng J., Liu X. Q., Wang C., et al. Erlotinib versus chemotherapy as first-line treatment for patients with advanced EGFR mutation-positive non-small-cell lung cancer (OPTIMAL, CTONG-0802): a multicentre, open-label, randomised, phase 3 study. *Lancet Oncol*. 2011;12(8):735-42.
4. Paz-Ares L., Soulieres D., Melezinek I., Moecks J., Keil L., Mok T., et al. Clinical outcomes in non-small-cell lung cancer patients with EGFR mutations: pooled analysis. *J Cell Mol Med*. 2010;14(1-2):51-69.
5. Cheng L., Alexander R. E., Maclennan G. T., Cummings O. W., Montironi R., Lopez-Beltran A., et al. Molecular pathology of lung cancer: key to personalized medicine. *Mod Pathol*. 2012;25(3):347-69.
6. TARCEVA® (erlotinib) Package Insert.
7. Wu Y. L., Lee J. S., Thongprasert S., Yu C. J., Zhang L., Ladrera G., et al. Intercalated combination of chemotherapy and erlotinib for patients with advanced stage non-small-cell lung cancer (FASTACT-2): a randomised, double-blind trial. *Lancet Oncol*. 2013;14(8):777-86.
8. TAGRISSO® (osimertinib) Package Insert.
9. Janne P. A., Yang J. C., Kim D. W., Planchard D., Ohe Y., Ramalingam S. S., et al. AZD9291 in EGFR inhibitor-resistant non-small-cell lung cancer. *N Engl J Med*. 2015;372(18):1689-99.
10. Soria J-C, Vansteenkiste J, Reungwetwantana T, et al. Osimertinib in Untreated EGFR-Mutated Advanced Non-Small-Cell Lung Cancer. *NEJM* 2018; 378:113-125.
11. Cohen MH, Williams GA, Sridhara R, Chen G, McGuinn WD, Jr, Morse D, et al. United States Food and Drug Administration Drug Approval summary: Gefitinib (ZD1839; Iressa) tablets. *Clin Cancer Res* 2004;10(4):1212-1218.
12. Mok TS, Wu YL, Thongprasert S, Yang CH, Chu S, Saijo, et al. Gefitinib or carboplatin-paclitaxel in pulmonary adenocarcinoma. *N Engl J Med* 2009;361(10):947-957.
13. Douillard J-Y, Ostoros G, Cobo M, Ciuleanu T, McCormack R, Webster A, et al. First-line gefitinib in Caucasian EGFR mutation-positive NSCLC patients: a phase-IV, open-label, single-arm study. *Br. J Ca* 2014;110:55-62.
14. Catalogue of Somatic Mutations in Cancer (COSMIC), 2011, v.51. <http://www.sanger.ac.uk/genetics/CGP/cosmic>.
15. Longo M. C., Berninger M. S., Hartley J. L. Use of uracil DNA glycosylase to control carry-over contamination in polymerase chain reactions. *Gene*. 1990;93(1):125-8.

16. Chosewood LC, Wilson DE. Biosafety and microbiological and biomedical laboratories-Fifth Edition. US Department of Health and Human Services Publication. (CDC). 2009:21-1112.
17. Clinical and Laboratory Standards Institute (CLSI). Protection of laboratory workers from occupationally acquired infections. Approved Guideline-Fourth Edition. CLSI Document M29-A4: Wayne, PA;CLSI, 2014.
18. International Air Transport Association. Dangerous Goods Regulations, 52nd Edition. 2011.
19. Costa D. B., Nguyen K. S., Cho B. C., Sequist L. V., Jackman D. M., Riely G. J., et al. Effects of erlotinib in EGFR mutated non-small cell lung cancers with resistance to gefitinib. *Clinical cancer research : an official journal of the American Association for Cancer Research*. 2008;14(21):7060-7.
20. Clinical and Laboratory Standards Institute (CLSI). Evaluation of Detection Capability for Clinical Laboratory Measurement Procedures; Approved Guideline - Second Edition. CLSI Document EP17-A2: Wayne, PA; CLSI, Jun 2012.
21. Clinical and Laboratory Standards Institute (CLSI). Interference testing in clinical chemistry; Approved Guideline-Second Edition. CLSI Document EP07-A2 Appendix D:Wayne, PA; CLSI, 2005.
22. Rosell R., Carcereny E., Gervais R., Vergnenegre A., Massuti B., Felip E., et al. Erlotinib versus standard chemotherapy as first-line treatment for European patients with advanced EGFR mutation-positive non-small-cell lung cancer (EURTAC): a multicentre, open-label, randomised phase 3 trial. *Lancet Oncol*. 2012;13(3):239-46.
23. Goss G., Tsai C. M., Shepherd F. A., Bazhenova L., Lee J. S., Chang G. C., et al. Osimertinib for pretreated EGFR Thr790Met-positive advanced non-small-cell lung cancer (AURA2): a multicentre, open-label, single-arm, phase 2 study. *The Lancet Oncology*. 2016;17(12):1643-52.
24. Clinical and Laboratory Standards Institute (CLSI). Evaluation of the linearity of quantitative measurement procedures: A statistical approach; Approved Guideline. CLSI Document EP-06A: Wayne, PA; CLSI, Apr 2003.

Document revision

Document Revision Information	
Doc Rev. 8.0 07/2023	Instrumentation and software required but not provided section in Section A and Section B updated the System Software version to 2.2 and added a note reference the Product Information Card. Updated cobas ® branding. Updated Trademarks and patents section, including the link. Please contact your local Roche Representative if you have any questions.