


COBAS[®] AmpliPrep Instrument

Addendum version 1.0 For use with the AMPLILINK Software





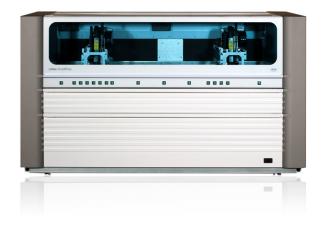

Publication information

Publication version	Revision date	Changes
1.0	September 2016	First version

Table 1

Revision history

Edition notice This addendum contains revisions to released COBAS AmpliPrep Instrument publications.



General attention

To avoid serious or fatal injury, ensure that you are familiar with the system and safety information before you use the system.

- ▶ Pay particular attention to all safety precautions.
- Always follow the instructions in this publication.
- ▶ Do not use the instrument in a way that is not described in this publication.
- ▶ Store all publications in a safe and easily retrievable place.

Copyright © 2016, F. Hoffmann-La Roche Ltd. All rights reserved.

Trademarks The following trademarks are acknowledged:

AMPLILINK, COBAS, AMPLIPREP, and TAQMAN are trademarks of Roche.

All other trademarks are the property of their respective owners.

Feedback Every effort has been made to ensure that this publication fulfills the intended use. All feedback on any aspect of this publication is welcome and is considered during updates. Contact your Roche representative, should you have any such feedback.

Contact addresses

•••	Roche Molecular Systems, Inc. 1080 US Highway 202 South
	Branchburg, NJ 08876
	USA
	Made in Switzerland
	Roche Diagnostics GmbH
EC REP	Sandhofer Strasse 116
	68305 Mannheim
	Germany

Roche Diagnostics

Table of contents


About the addendum content	4
Revisions to COBAS [*] AmpliPrep Instrument publications	5
Revision 1: Addition of RoHS directive and update of CE compliance	
Revision 2: Addition of information about a fluorinated greenhouse gas	
Revision 3: Addition of print quality details for barcodes	

Roche Diagnostics

About the addendum content

Roche recommends that you familiarize yourself with the new and/or revised content provided in this addendum.

The following illustration explains how this content is presented in this document.

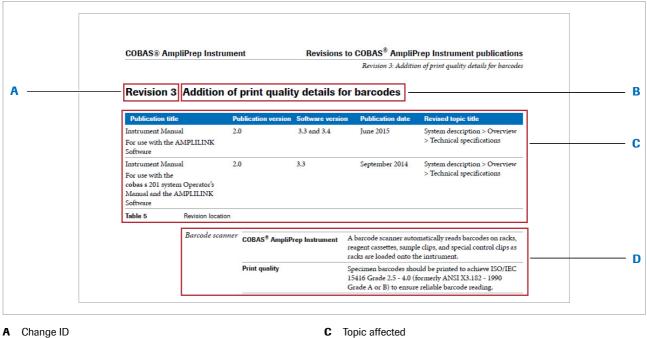

B Change summary

- C Topic affected
- **D** Changed element

Figure 1 Structure of a revision

-ý- If you print these pages, Roche recommends printing them single-sided. In this way, you can easily insert the new and/or revised content in its appropriate location(s) in the existing document.

Roche Diagnostics

Revision 1: Addition of RoHS directive and update of CE compliance

Revisions to COBAS[®] AmpliPrep Instrument publications

Revision 1: Addition of RoHS directive and update of CE compliance

Publication title	Publication version	Software version	Publication date	Revised topic title
Instrument Manual	2.0	3.3 and 3.4	June 2015	Publication information
For use with the AMPLILINK Software				
Instrument Manual	2.0	3.3	September 2014	Publication information
For use with the cobas s 201 system Operator's Manual and the AMPLILINK Software				

Table 2 Revision location


Approvals The COBAS® AmpliPrep Instrument meets the requirements laid down in:

Directive 98/79/EC of the European Parliament and of the Council of 27 October 1998 on in vitro diagnostic medical devices.

Directive 2011/65/EU of the European Parliament and of the Council of 8 June 2011 on the restriction of the use of certain hazardous substances in electrical and electronic equipment.

Compliance is provided by means of the Declaration of Conformity.

The following marks demonstrate compliance:

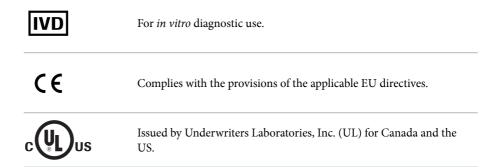

Roche Diagnostics

Revision 2: Addition of information about a fluorinated greenhouse gas

Revision 2: Addition of information about a fluorinated greenhouse gas

Publication title	Publication version	Software version	Publication date	Revised topic title
Instrument Manual	2.0	3.3 and 3.4	June 2015	Publication information
For use with the AMPLILINK Software				
T.I. 6 D.: 1 ::				

Table 3 Revision location

Fluorinated greenhouse gas The product contains a fluorinated greenhouse gas in the hermetically sealed refrigeration.

Туре	Charge weight (kg)	CO ₂ equivalent (tonne)	Global warming potential
R134a	0.200	0.286	1430

 Table 4
 Fluorinated greenhouse gas detail

Roche Diagnostics

Revision 3: Addition of print quality details for barcodes

Revision 3: Addition of print quality details for barcodes

Publication tit	le I	Publication version	Software version	n Publication date	Revised topic title	
Instrument Man	nual 2	2.0	3.3 and 3.4	June 2015	System description > Overview	
For use with the Software	AMPLILINK				> Technical specifications	
Instrument Man	nual 2	2.0	3.3	September 2014	System description > Overview	
For use with the	!				> Technical specifications	
cobas s 201 syste	em Operator's					
Manual and the	AMPLILINK					
Software						
Table 5	Revision location					
	Barcode scanner COBAS® AmpliPrep Instrument		A barcode scanner automatically reads barcodes on racks, reagent cassettes, sample clips, and special control clips as racks are loaded onto the instrument.			
		Print quality		Specimen barcodes should be printed to achieve ISO/IEC 15416 Grade 2.5 - 4.0 (formerly ANSI X3.182 - 1990 Grade A or B) to ensure reliable barcode reading.		

Roche Diagnostics