



# COBAS<sup>®</sup> TaqMan<sup>®</sup> 48 Analyzer

Addendum version 1.0

For use with the AMPLILINK Software



**cobas<sup>®</sup>**  
*Life needs answers*

## Publication information

Publication version	Revision date	Changes
1.0	September 2016	First version

**Table 1** Revision history

*Edition notice* This addendum contains revisions to released COBAS® TaqMan® 48 Analyzer publications.



### General attention

To avoid serious or fatal injury, ensure that you are familiar with the system and safety information before you use the system.

- ▶ Pay particular attention to all safety precautions.
- ▶ Always follow the instructions in this publication.
- ▶ Do not use the instrument in a way that is not described in this publication.
- ▶ Store all publications in a safe and easily retrievable place.

*Copyright* © 2016, F. Hoffmann-La Roche Ltd. All rights reserved.

*Trademarks* The following trademarks are acknowledged:

AMPLILINK, AMPERASE, COBAS, AMPLIPREP, and TAQMAN are trademarks of Roche.


All other trademarks are the property of their respective owners.

*Feedback* Every effort has been made to ensure that this publication fulfills the intended use. All feedback on any aspect of this publication is welcome and is considered during updates. Contact your Roche representative, should you have any such feedback.

## Contact addresses



Roche Molecular Systems, Inc.  
1080 US Highway 202 South  
Branchburg, NJ 08876  
USA  
Made in Switzerland



Roche Diagnostics GmbH  
Sandhofer Strasse 116  
68305 Mannheim  
Germany

**Table of contents**

About the addendum content.....5


Revisions to COBAS® TaqMan® 48 Analyzer publications .....6

    Revision 1: Addition of RoHS directive and update of CE compliance.....6

## About the addendum content

Roche recommends that you familiarize yourself with the new and/or revised content provided in this addendum.

The following illustration explains how this content is presented in this document.

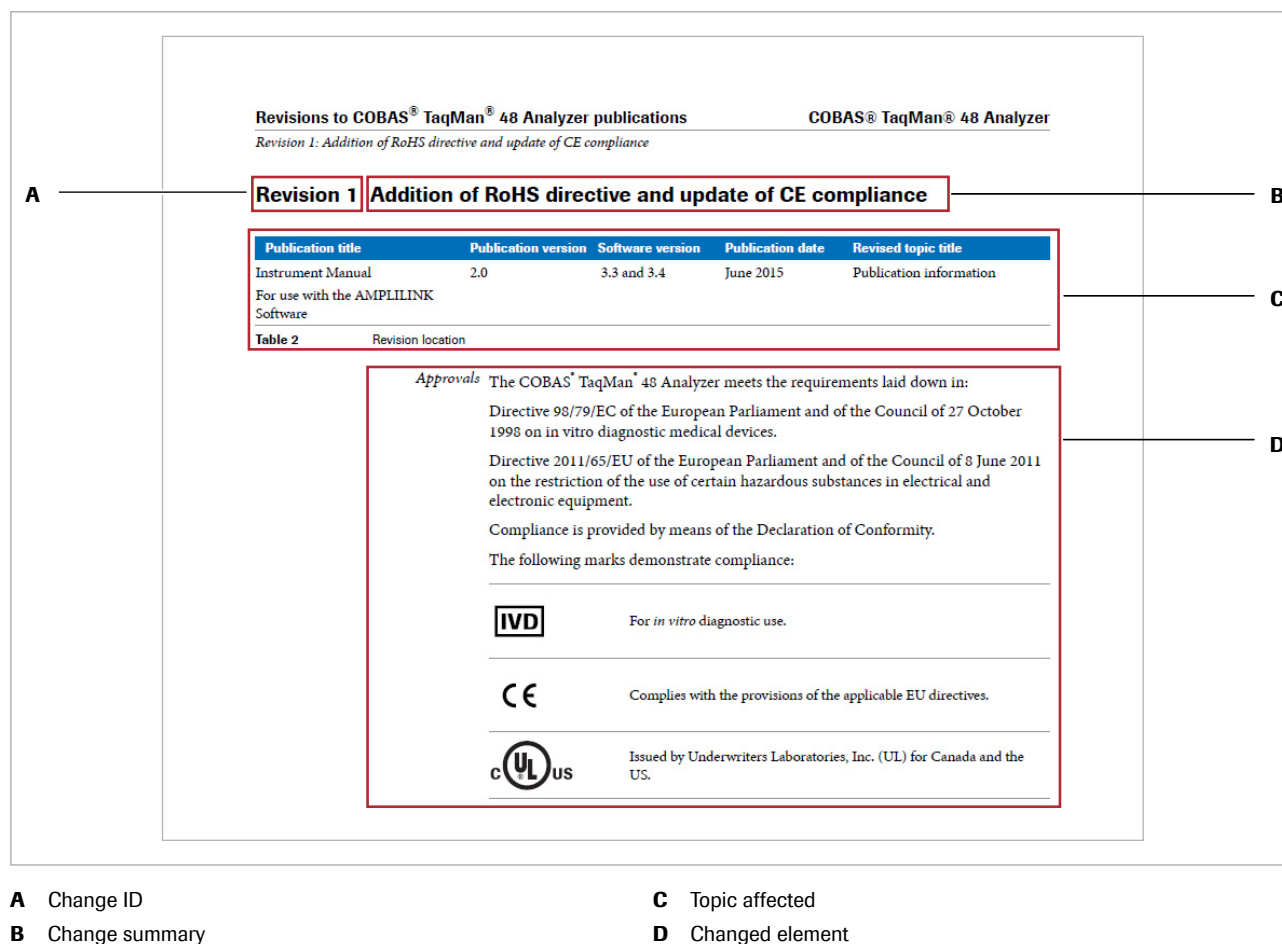

**Figure 1** Structure of a revision

☞ If you print these pages, Roche recommends printing them single-sided. In this way, you can easily insert the new and/or revised content in its appropriate location(s) in the existing document.

## Revisions to COBAS® TaqMan® 48 Analyzer publications

### Revision 1: Addition of RoHS directive and update of CE compliance

Publication title	Publication version	Software version	Publication date	Revised topic title
Instrument Manual For use with the AMPLILINK Software	2.0	3.3 and 3.4	June 2015	Publication information

**Table 2** Revision location

*Approvals* The COBAS® TaqMan® 48 Analyzer meets the requirements laid down in:

Directive 98/79/EC of the European Parliament and of the Council of 27 October 1998 on in vitro diagnostic medical devices.

Directive 2011/65/EU of the European Parliament and of the Council of 8 June 2011 on the restriction of the use of certain hazardous substances in electrical and electronic equipment.

Compliance is provided by means of the Declaration of Conformity.

The following marks demonstrate compliance:



For *in vitro* diagnostic use.



Complies with the provisions of the applicable EU directives.



Issued by Underwriters Laboratories, Inc. (UL) for Canada and the US.

